

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103018\
 Data File : PO050755.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2018 13:30
 Operator : SM/SJ
 Sample : J5707-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DS-T1-BASE-CON

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 00:42:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.355	3.347	10256500	4513318	20.519	20.765
2) SA Decachlor...	10.014	8.095	5555141	4124137	17.872	16.123

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103018\
Data File : PO050755.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2018 13:30
Operator : SM/SJ
Sample : J5707-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DS-T1-BASE-CON

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 00:42:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

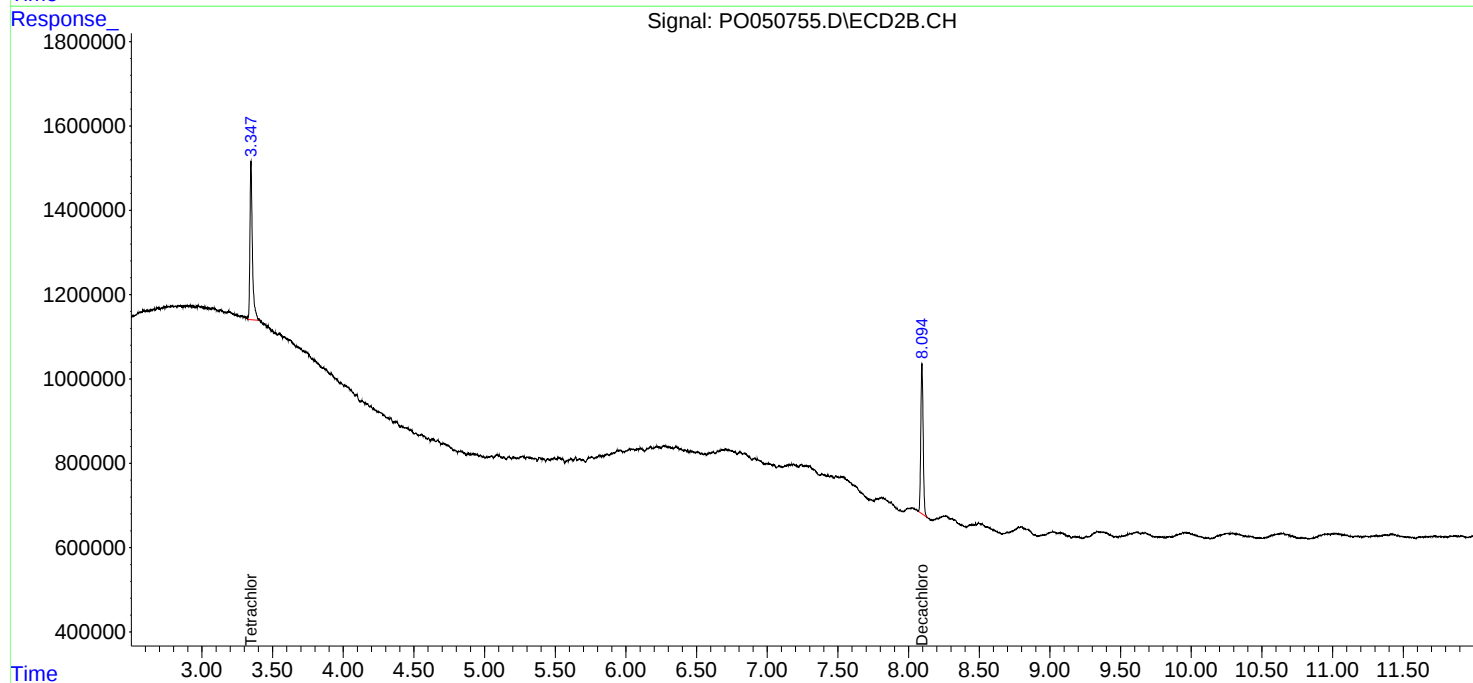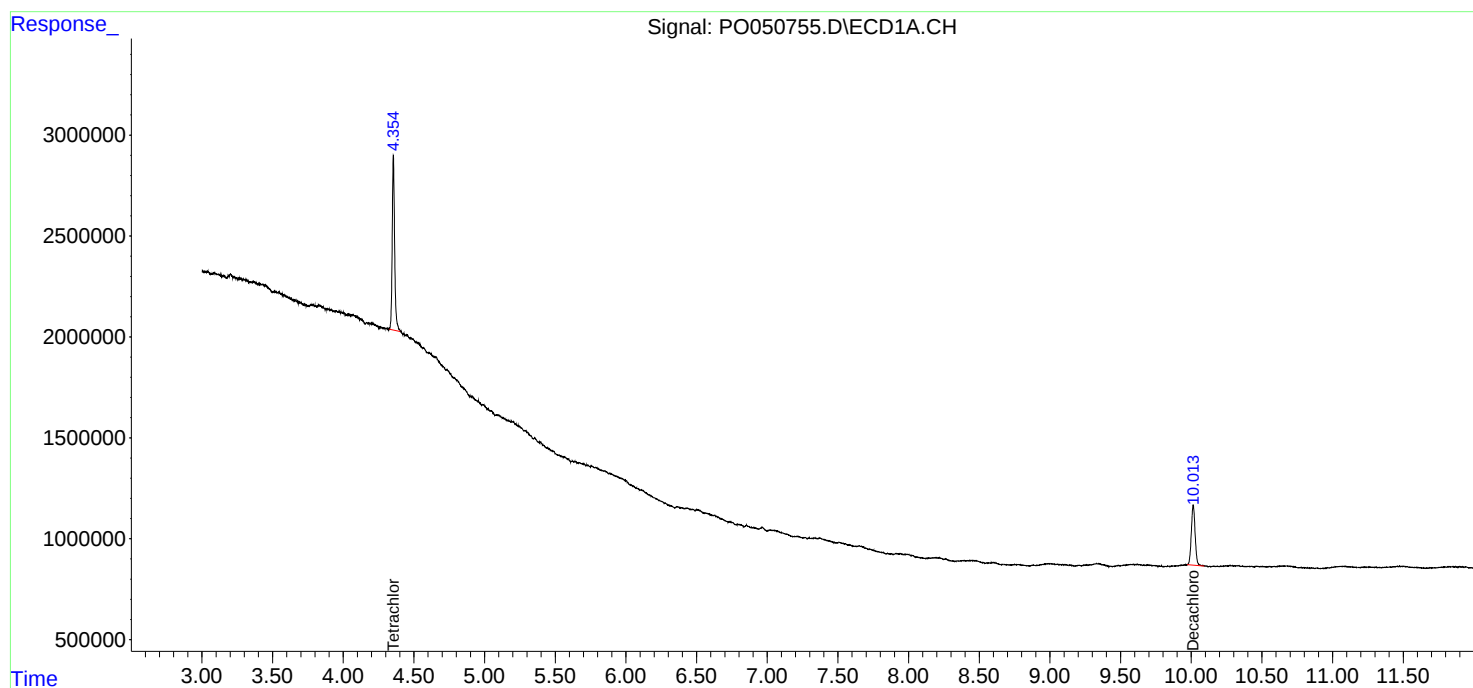


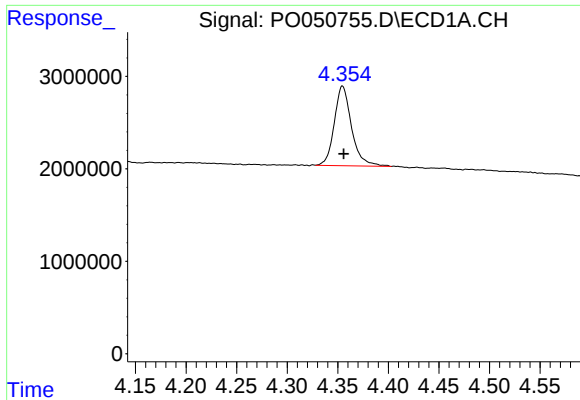

#1 Tetrachloro-m-xylene


R.T.: 4.355 min
Delta R.T.: -0.001 min
Response: 10256500
Conc: 20.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
DS-T1-BASE-CON

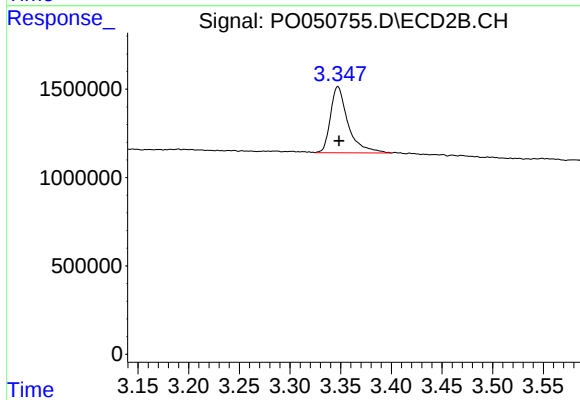


#1 Tetrachloro-m-xylene

R.T.: 3.347 min
Delta R.T.: -0.001 min
Response: 4513318
Conc: 20.76 ng/ml

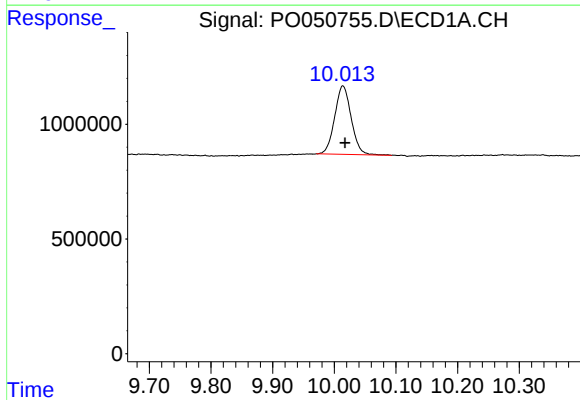

#2 Decachlorobiphenyl

R.T.: 10.014 min
Delta R.T.: -0.004 min
Response: 5555141
Conc: 17.87 ng/ml

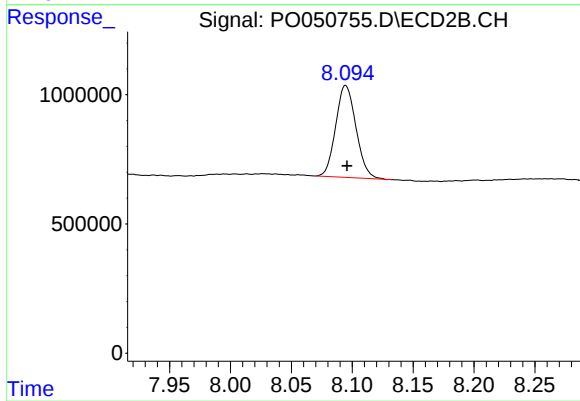

#2 Decachlorobiphenyl

R.T.: 8.095 min
Delta R.T.: -0.001 min
Response: 4124137
Conc: 16.12 ng/ml