

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103018\
 Data File : P0050756.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 30 Oct 2018 13:47
 Operator : SM/SJ
 Sample : J5697-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CHRT-58-66-98-92

Manual Integrations
 APPROVED

Sohil
 10/31/2018 3:20:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 00:47:09 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Oct 30 07:48:38 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.355	3.347	7317042	3465895	14.638	15.946m
2) SA Decachlor...	10.014	8.094	3997176	3214617	12.860	12.568

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103018\
Data File : PO050756.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 30 Oct 2018 13:47
Operator : SM/SJ
Sample : J5697-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CHRT-58-66-98-92


Manual Integrations
APPROVED

Sohil
10/31/2018 3:20:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 00:47:09 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Oct 30 07:48:38 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

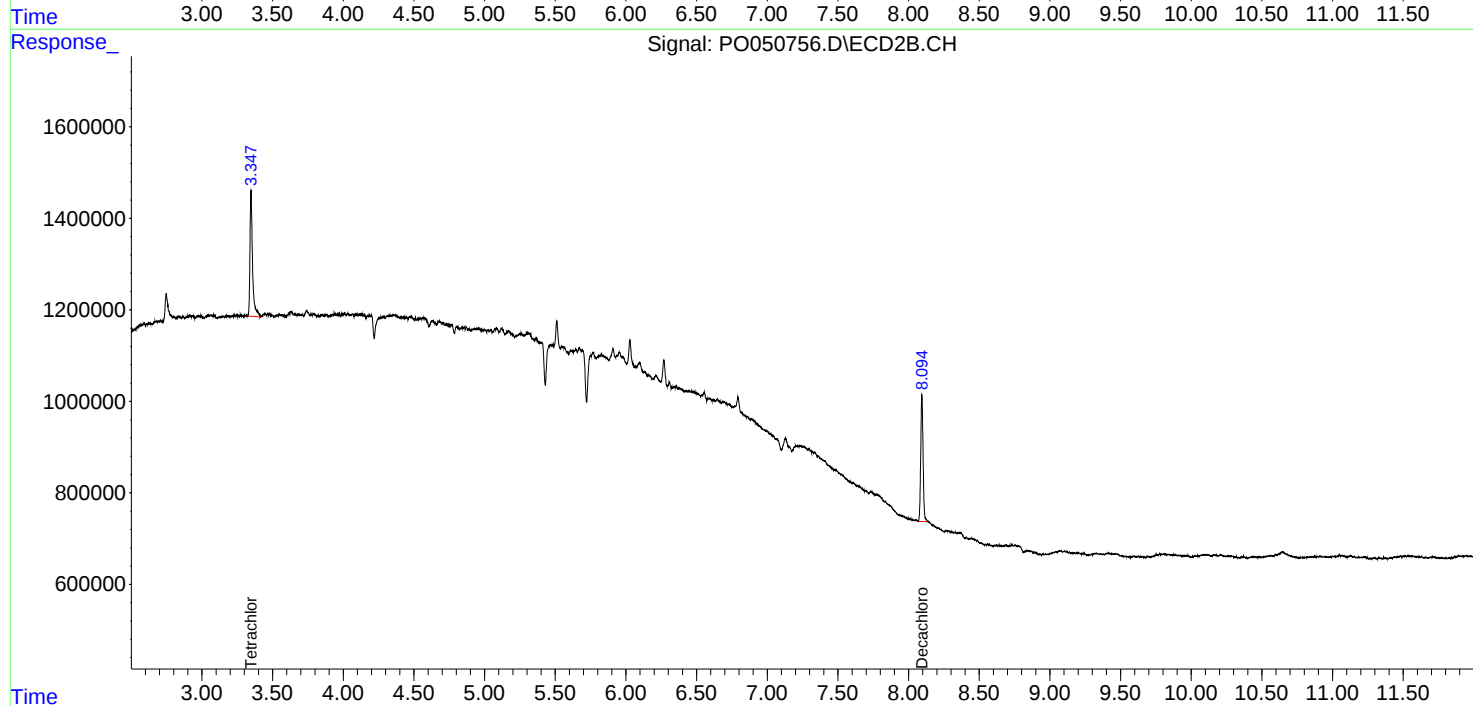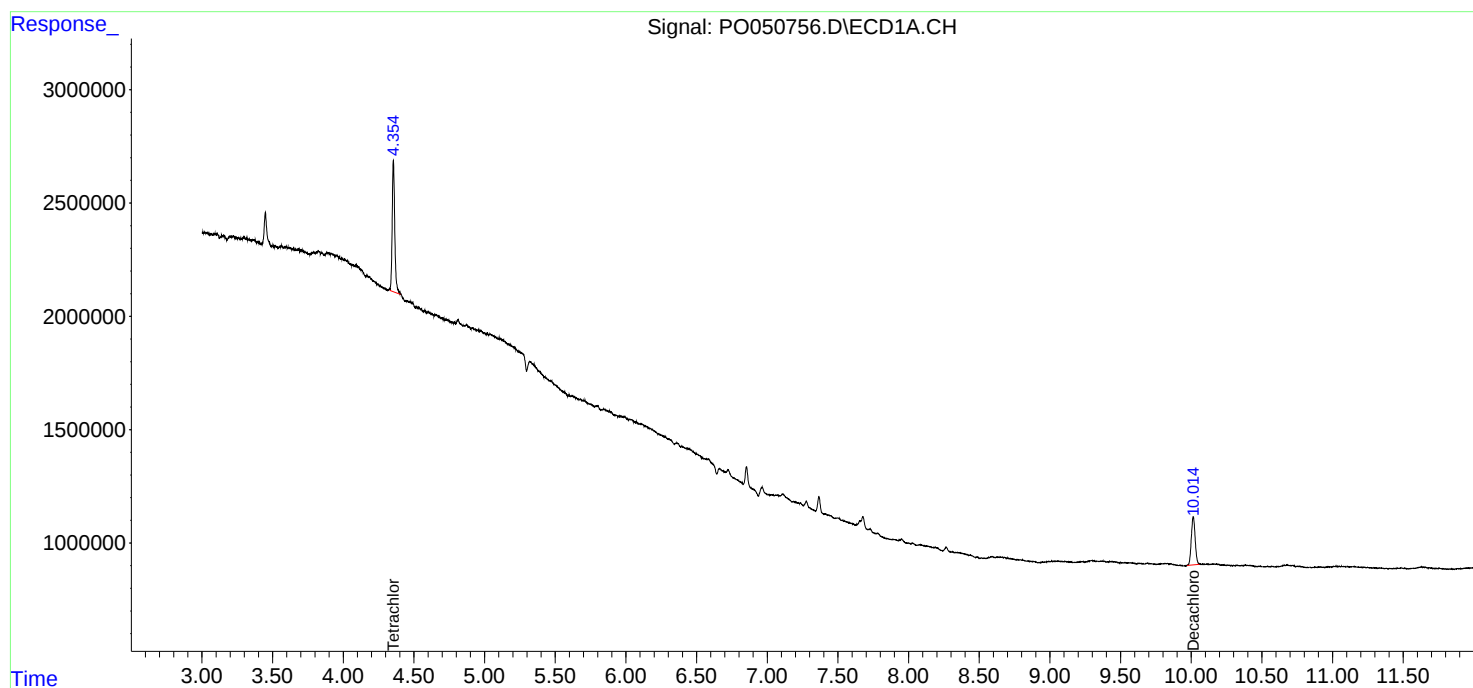

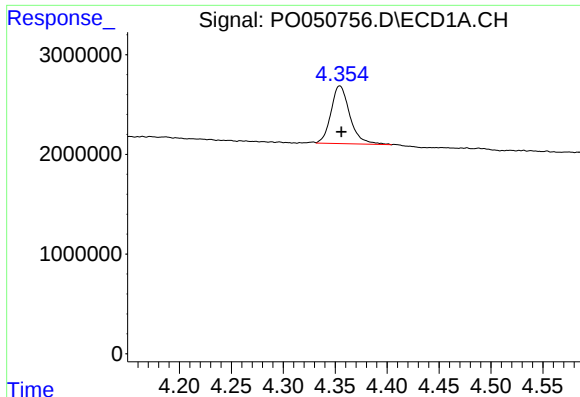


#1 Tetrachloro-m-xylene

R.T.: 4.355 min
Delta R.T.: -0.001 min
Response: 7317042
Conc: 14.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
CHRT-58-66-98-92


Manual Integrations
APPROVED

Sohil
10/31/2018 3:20:01 PM

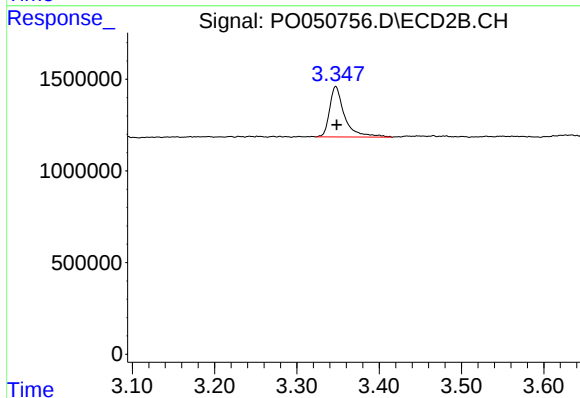


#1 Tetrachloro-m-xylene

R.T.: 3.347 min
Delta R.T.: -0.001 min
Response: 3465895
Conc: 15.95 ng/ml m

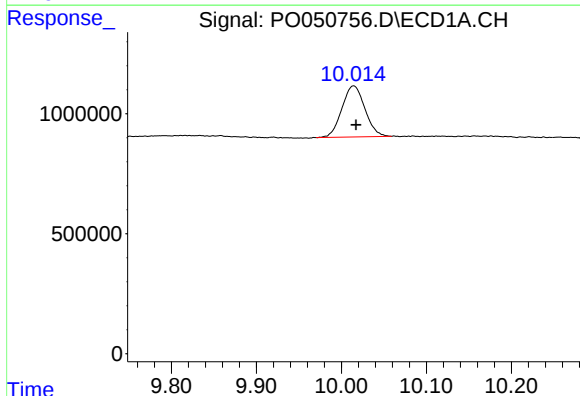

#2 Decachlorobiphenyl

R.T.: 10.014 min
Delta R.T.: -0.003 min
Response: 3997176
Conc: 12.86 ng/ml

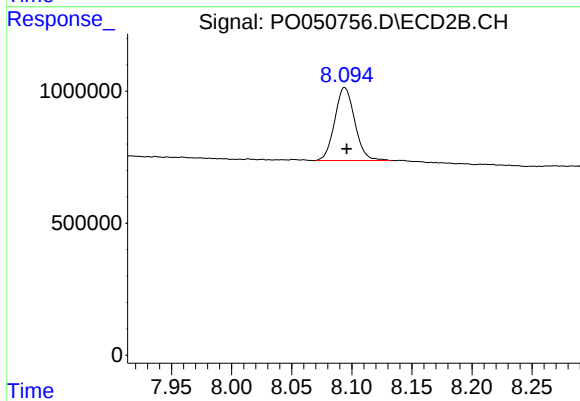

#2 Decachlorobiphenyl

R.T.: 8.094 min
Delta R.T.: -0.002 min
Response: 3214617
Conc: 12.57 ng/ml