

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103119\
 Data File : P0063374.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Oct 2019 20:11
 Operator : HP/AJ
 Sample : K5620-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-26A-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 01:18:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.316	3.481	1296804	1302371	22.251	23.847
2)	SA Decachlor...	9.934	8.320	1064520	709057	18.296	16.585
Target Compounds							
7)	L1 AR-1016-5	0.000	4.903	0	9974	N.D.	6.621 #
10)	L2 AR-1221-3	0.000	3.883	0	27582	N.D.	22.432 #
11)	L3 AR-1232-1	0.000	3.883	0	27582	N.D.	16.160 #
15)	L3 AR-1232-5	0.000	4.903	0	9974	N.D.	10.657 #
20)	L4 AR-1242-5	0.000	5.297	0	22386	N.D.	16.024 #
24)	L5 AR-1248-4	0.000	4.903	0	9974	N.D.	5.539 #
25)	L5 AR-1248-5	0.000	5.338	0	8361	N.D.	4.523 #
26)	L6 AR-1254-1	0.000	5.297	0	22386	N.D.	7.431 #
27)	L6 AR-1254-2	0.000	5.491	0	107180	N.D.	39.740 #
28)	L6 AR-1254-3	0.000	5.831	0	27797	N.D.	6.475 #
30)	L6 AR-1254-5	0.000	6.465	0	120911	N.D.	32.436 #
32)	L7 AR-1260-2	0.000	6.144	0	28840	N.D.	7.517 #
34)	L7 AR-1260-4	0.000	6.754	0	23941	N.D.	9.456 #
35)	L7 AR-1260-5	0.000	6.995	0	78966	N.D.	12.955 #
36)	L8 AR-1262-1	0.000	6.507	0	28945	N.D.	15.908 #
37)	L8 AR-1262-2	0.000	6.995	0	78966	N.D.	11.080 #
38)	L8 AR-1262-3	0.000	7.335	0	21275	N.D.	7.938 #
39)	L8 AR-1262-4	0.000	7.335	0	21275	N.D.	4.639 #
40)	L8 AR-1262-5	0.000	7.868	0	3189	N.D.	1.625 #
41)	L9 AR-1268-1	0.000	7.335	0	21275	N.D.	2.670 #
42)	L9 AR-1268-2	0.000	7.335	0	21275	N.D.	3.231 #
44)	L9 AR-1268-4	0.000	7.868	0	3189	N.D.	1.477 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103119\
Data File : PO063374.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2019 20:11
Operator : HP/AJ
Sample : K5620-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampled :
TP-26A-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 01:18:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

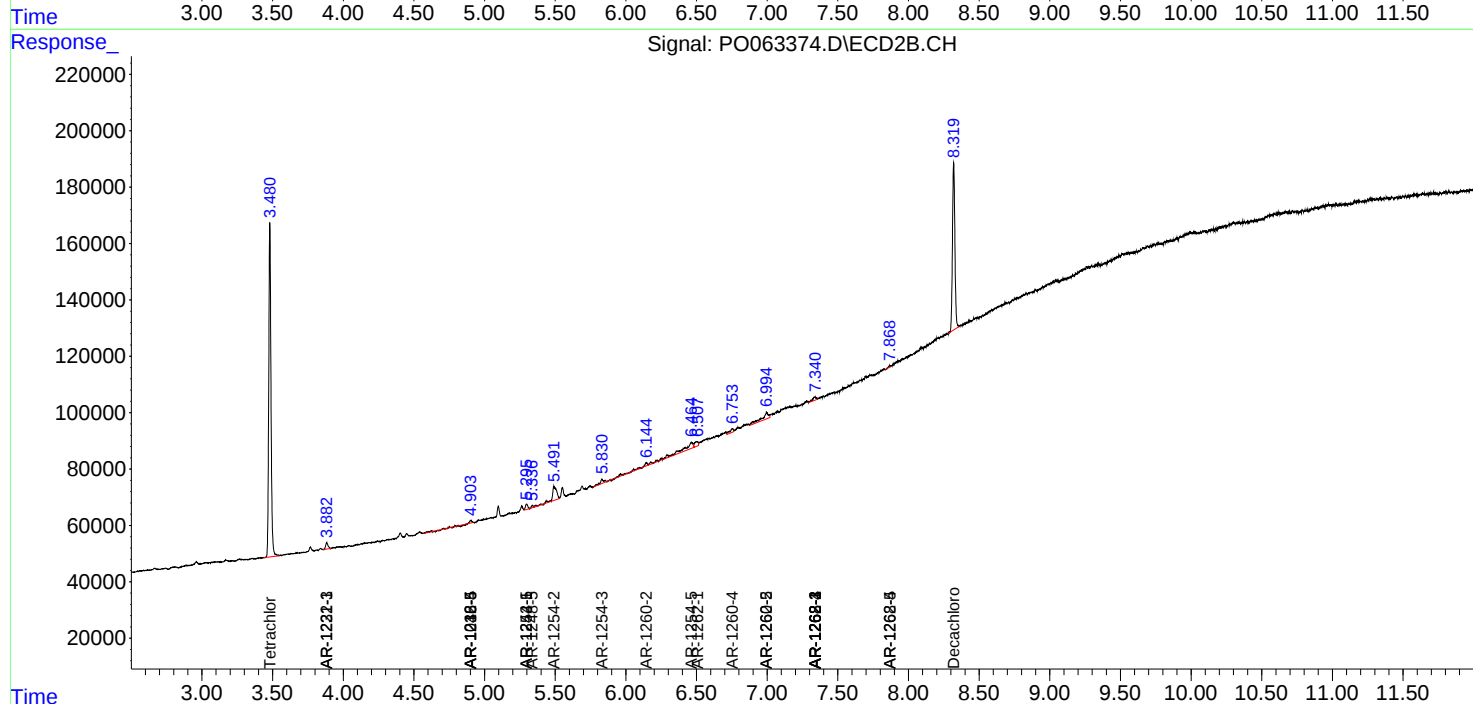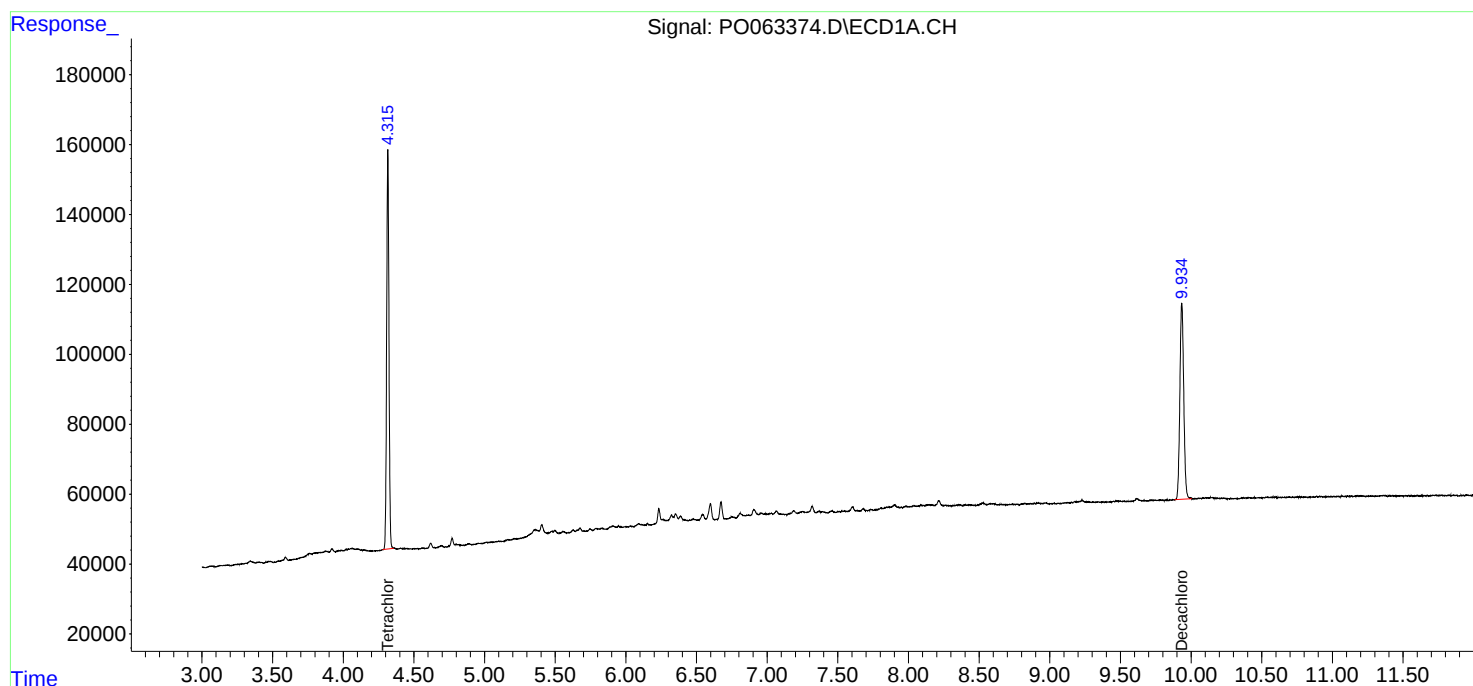


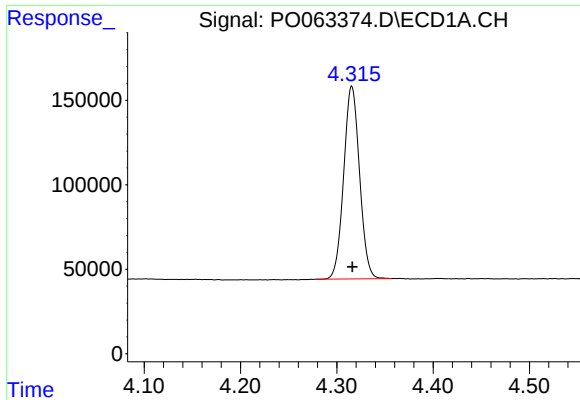

#1 Tetrachloro-m-xylene


R.T.: 4.316 min
Delta R.T.: 0.000 min
Response: 1296804
Conc: 22.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

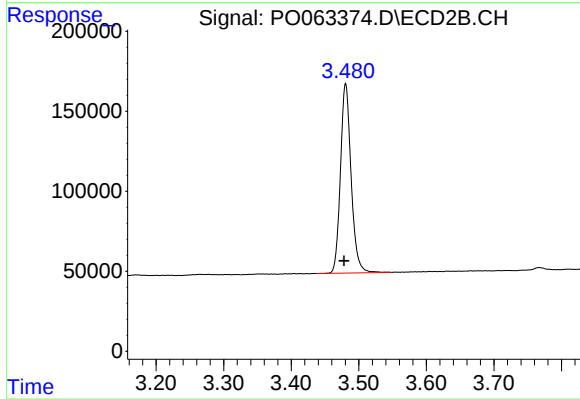


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.003 min
Response: 1302371
Conc: 23.85 ng/ml

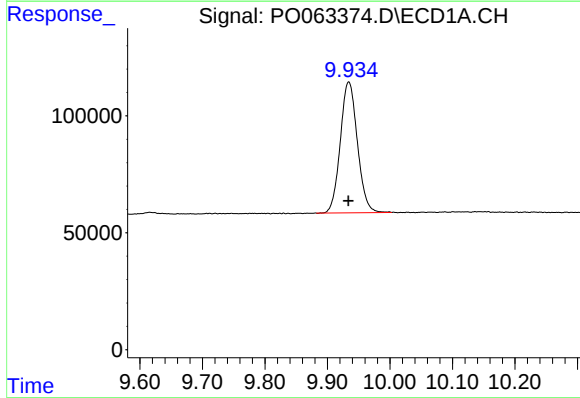


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: 0.000 min
Response: 1064520
Conc: 18.30 ng/ml

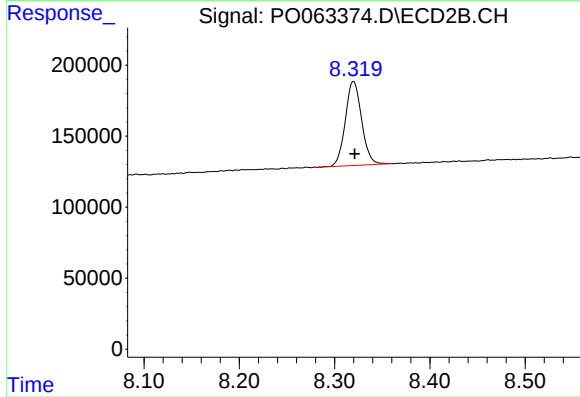

#2 Decachlorobiphenyl


R.T.: 8.320 min
Delta R.T.: -0.001 min
Response: 709057
Conc: 16.59 ng/ml

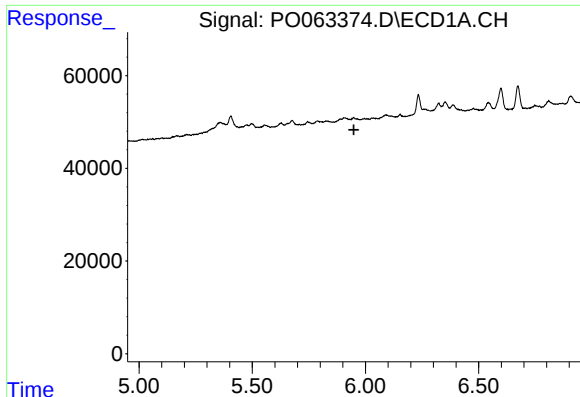

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 5.949 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

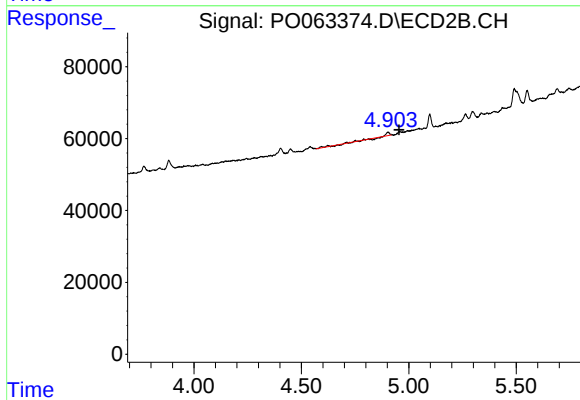


#7 AR-1016-5

R.T.: 4.903 min
Delta R.T.: -0.052 min
Response: 9974
Conc: 6.62 ng/ml

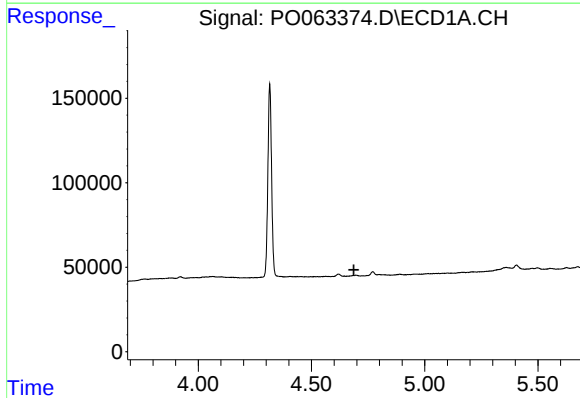


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T.: 4.687 min
Response: 0
Conc: N.D.

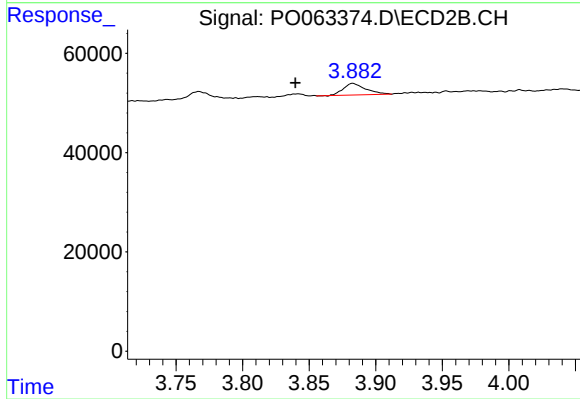

#10 AR-1221-3


R.T.: 3.883 min
Delta R.T.: 0.043 min
Response: 27582
Conc: 22.43 ng/ml

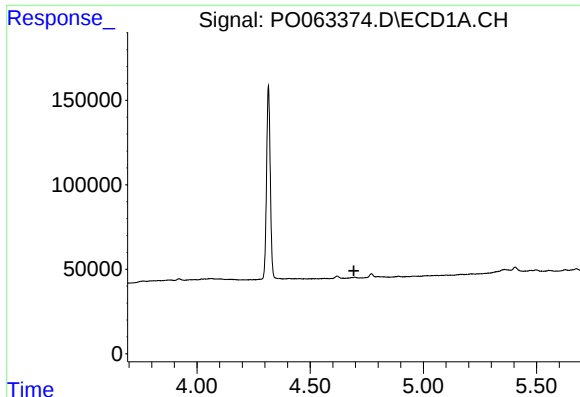

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 4.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

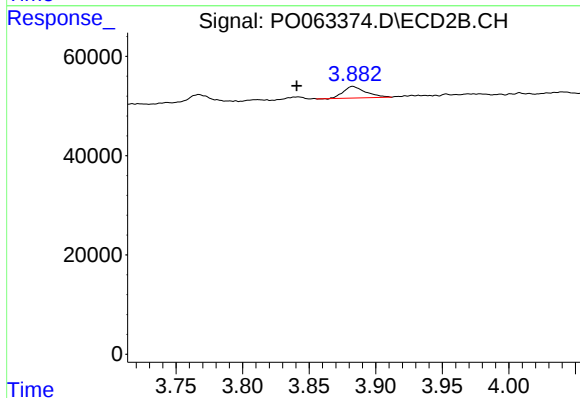


#11 AR-1232-1

R.T.: 3.883 min
Delta R.T.: 0.042 min
Response: 27582
Conc: 16.16 ng/ml

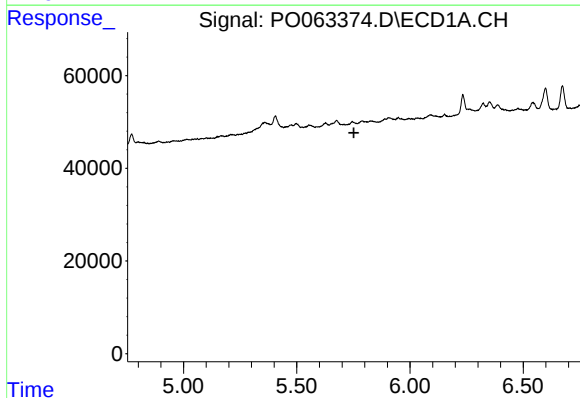


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.753 min
Response: 0
Conc: N.D.

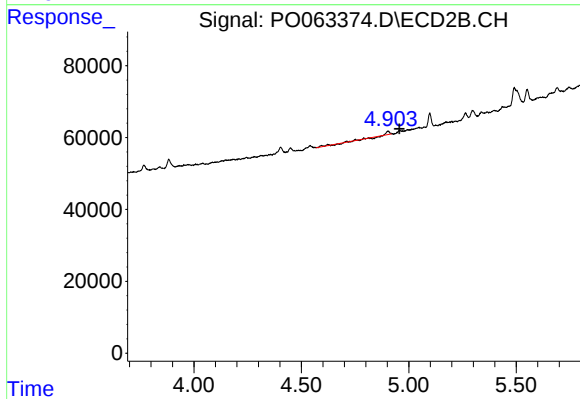

#15 AR-1232-5


R.T.: 4.903 min
Delta R.T.: -0.054 min
Response: 9974
Conc: 10.66 ng/ml

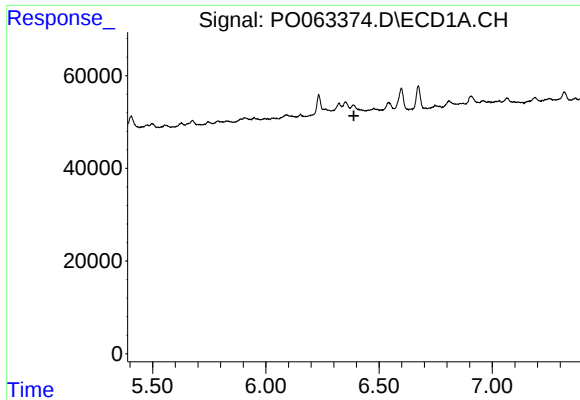

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T.: 6.389 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

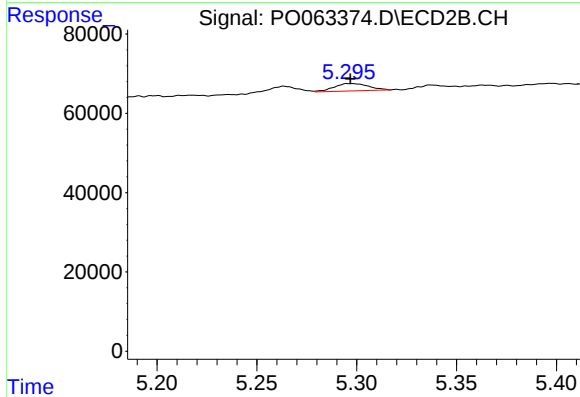


#20 AR-1242-5

R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 22386
Conc: 16.02 ng/ml

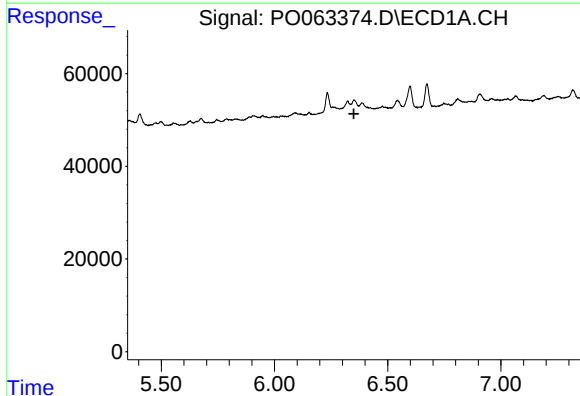


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T.: 6.351 min
Response: 0
Conc: N.D.

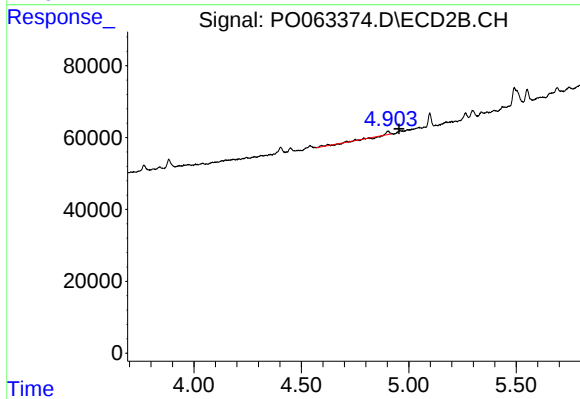

#24 AR-1248-4


R.T.: 4.903 min
Delta R.T.: -0.052 min
Response: 9974
Conc: 5.54 ng/ml

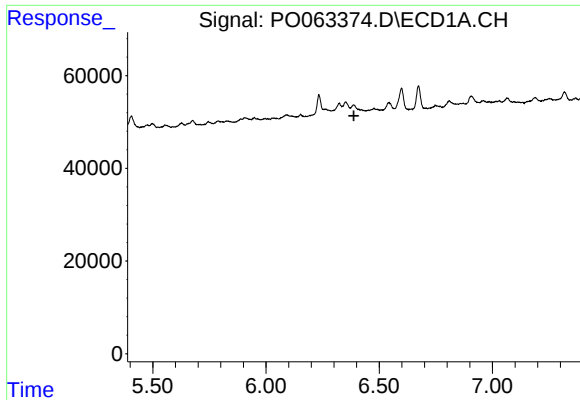

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 6.388 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

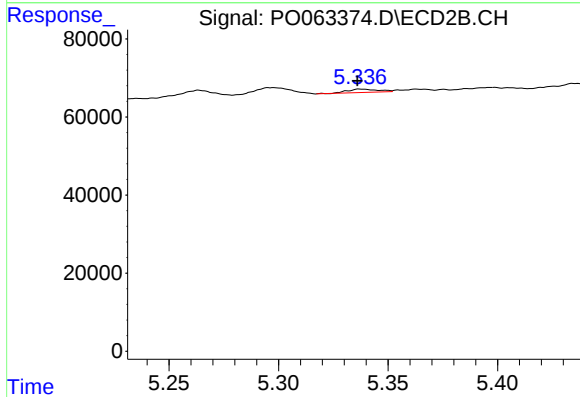


#25 AR-1248-5

R.T.: 5.338 min
Delta R.T.: 0.002 min
Response: 8361
Conc: 4.52 ng/ml

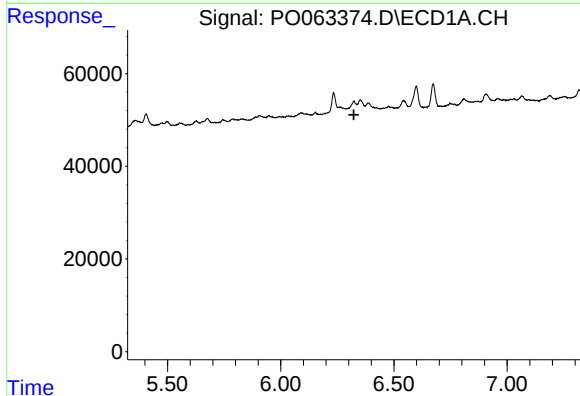


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 6.323 min
Response: 0
Conc: N.D.

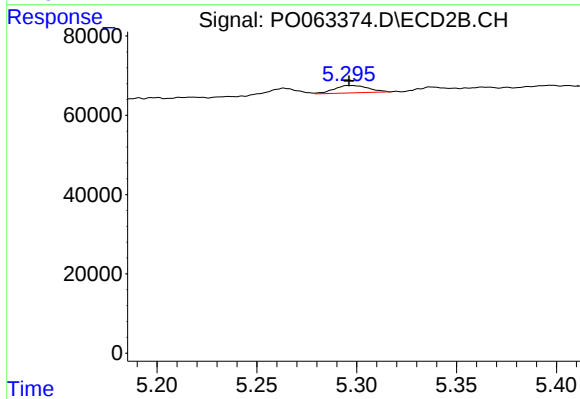

#26 AR-1254-1


R.T.: 5.297 min
Delta R.T.: 0.000 min
Response: 22386
Conc: 7.43 ng/ml

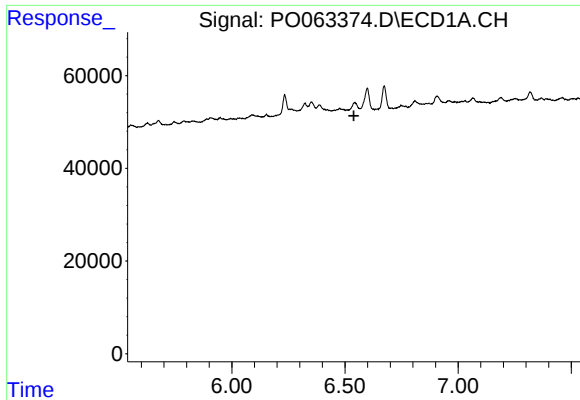

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 6.539 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

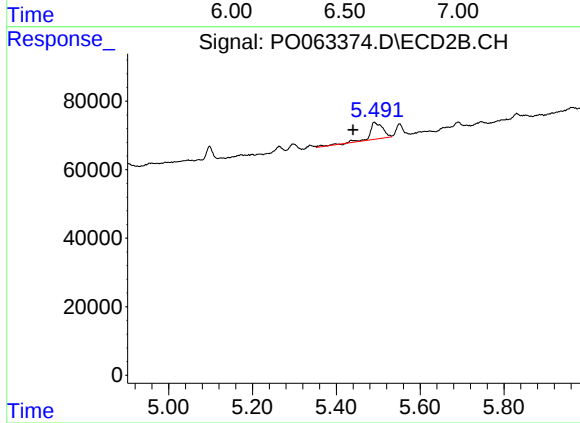


#27 AR-1254-2

R.T.: 5.491 min
Delta R.T.: 0.050 min
Response: 107180
Conc: 39.74 ng/ml

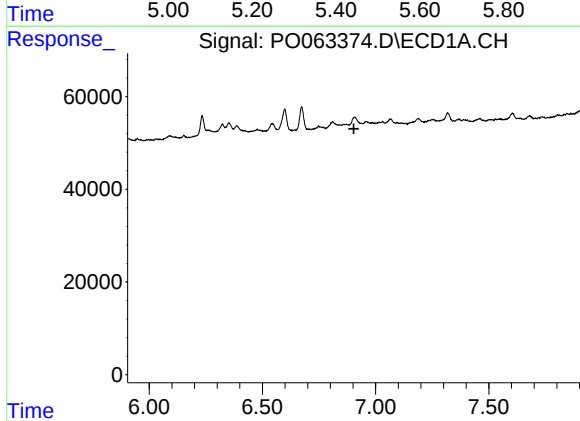


#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.904 min
Response: 0
Conc: N.D.

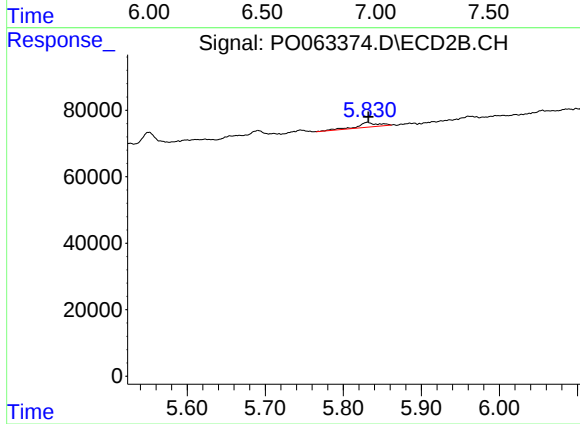

#28 AR-1254-3


R.T.: 5.831 min
Delta R.T.: -0.002 min
Response: 27797
Conc: 6.47 ng/ml

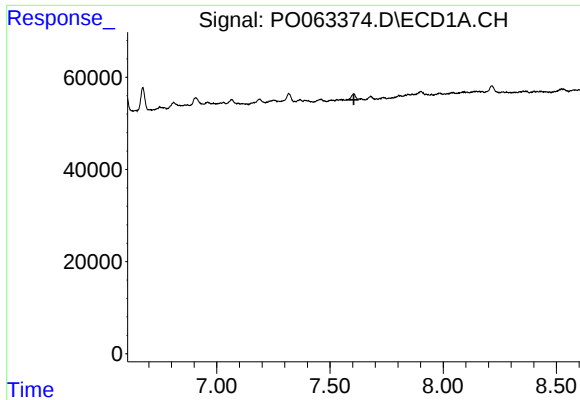

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 7.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

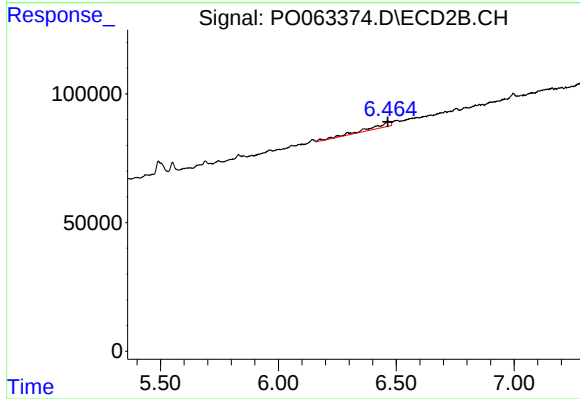


#30 AR-1254-5

R.T.: 6.465 min
Delta R.T.: 0.000 min
Response: 120911
Conc: 32.44 ng/ml

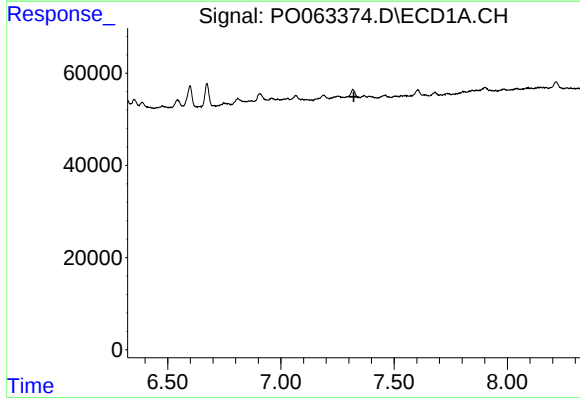


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.322 min
Response: 0
Conc: N.D.

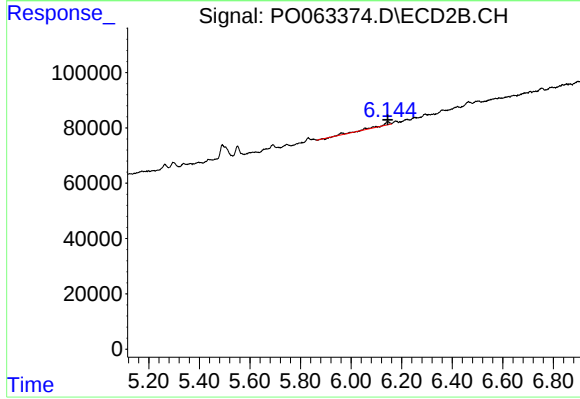

#32 AR-1260-2


R.T.: 6.144 min
Delta R.T.: 0.000 min
Response: 28840
Conc: 7.52 ng/ml

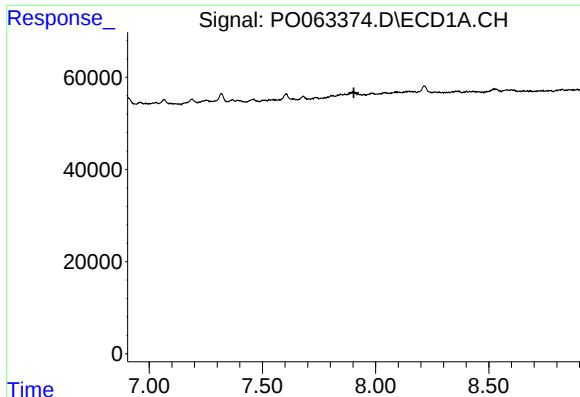

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.904 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

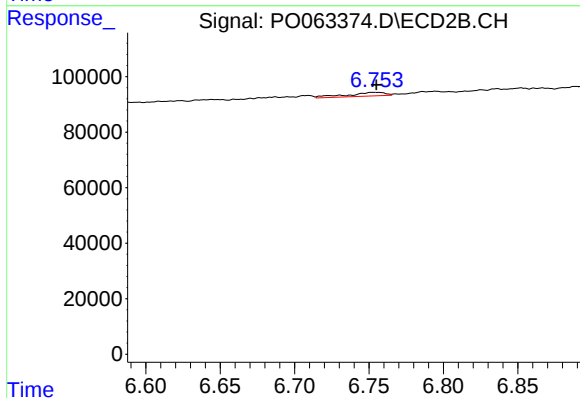


#34 AR-1260-4

R.T.: 6.754 min
Delta R.T.: -0.001 min
Response: 23941
Conc: 9.46 ng/ml

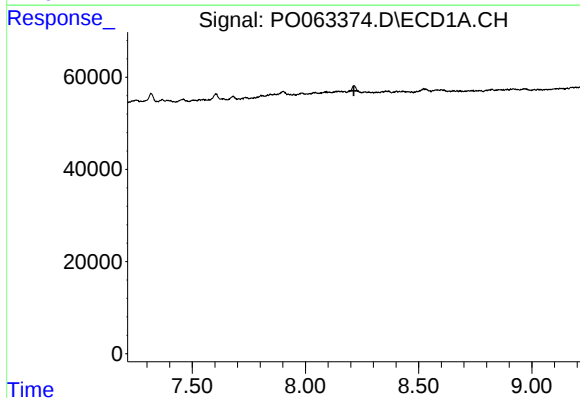


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.214 min
Response: 0
Conc: N.D.

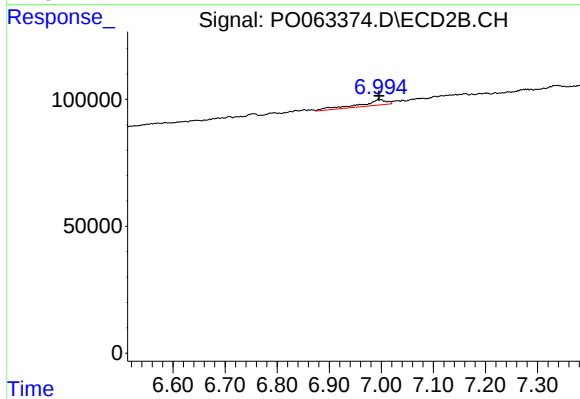

#35 AR-1260-5


R.T.: 6.995 min
Delta R.T.: 0.000 min
Response: 78966
Conc: 12.96 ng/ml

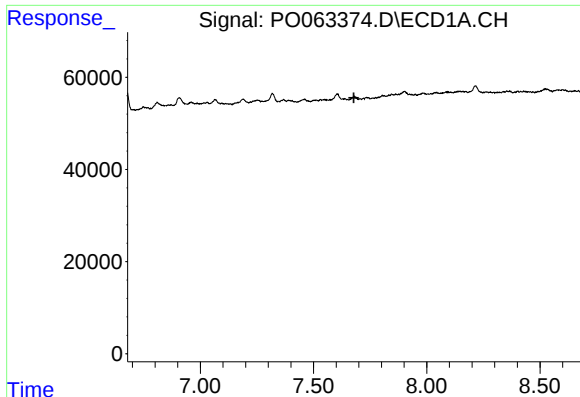

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 7.678 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

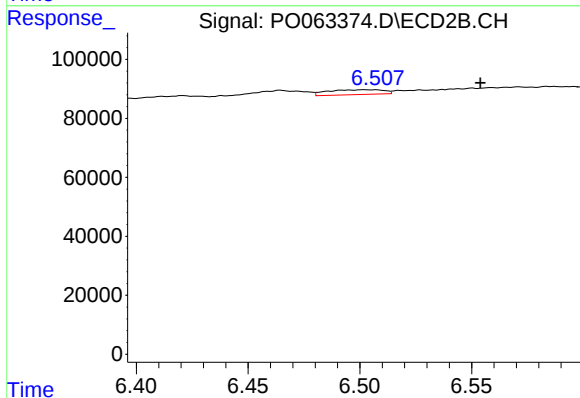


#36 AR-1262-1

R.T.: 6.507 min
Delta R.T.: -0.047 min
Response: 28945
Conc: 15.91 ng/ml

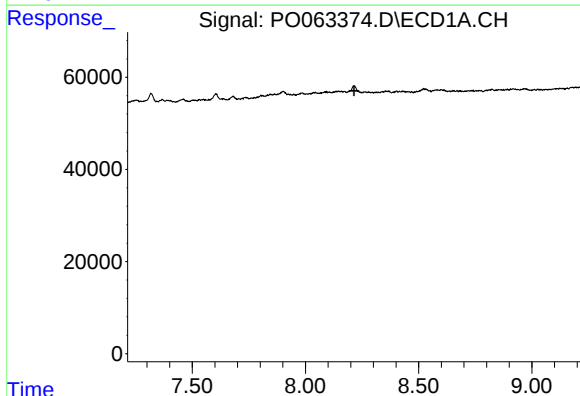


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.214 min
Response: 0
Conc: N.D.

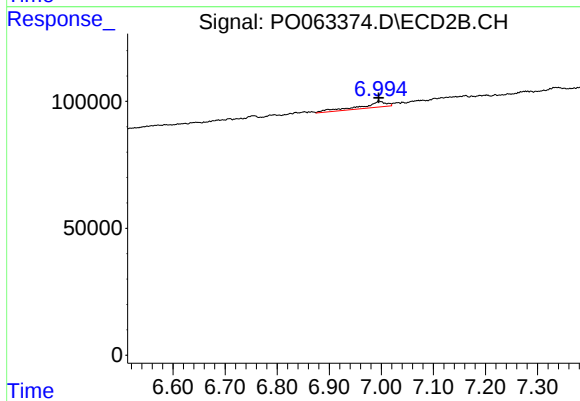

#37 AR-1262-2


R.T.: 6.995 min
Delta R.T.: 0.000 min
Response: 78966
Conc: 11.08 ng/ml

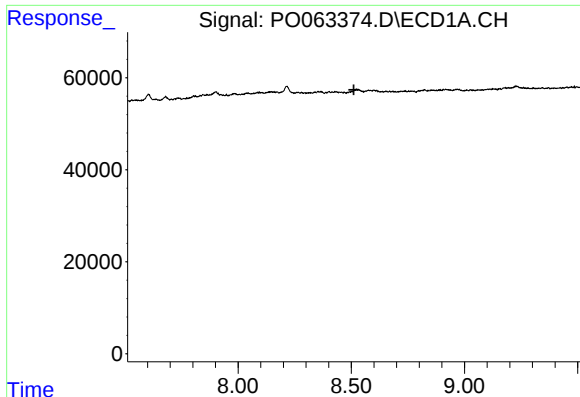

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 8.512 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

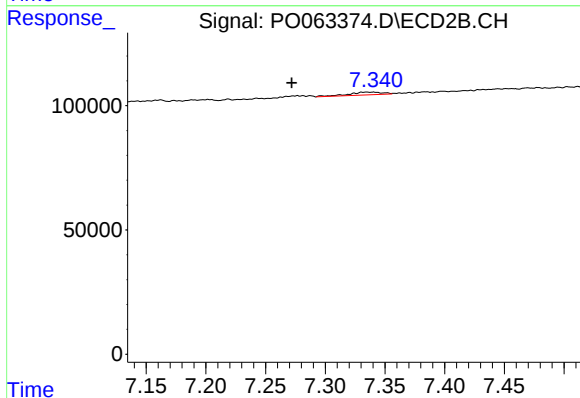


#38 AR-1262-3

R.T.: 7.335 min
Delta R.T.: 0.063 min
Response: 21275
Conc: 7.94 ng/ml

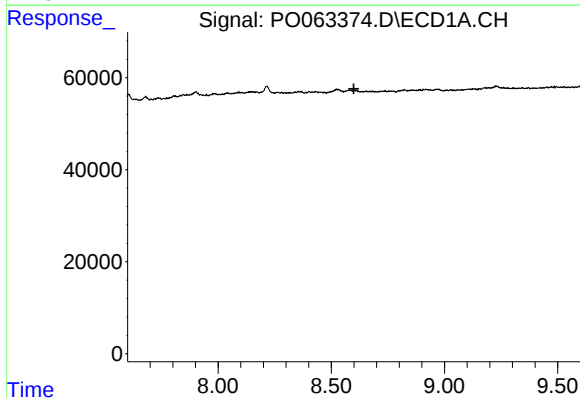


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.600 min
Response: 0
Conc: N.D.

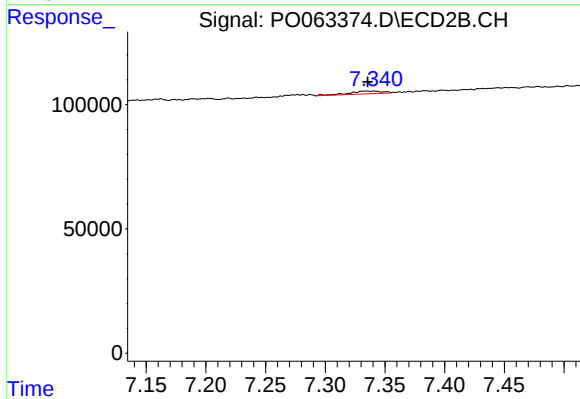

#39 AR-1262-4


R.T.: 7.335 min
Delta R.T.: -0.001 min
Response: 21275
Conc: 4.64 ng/ml

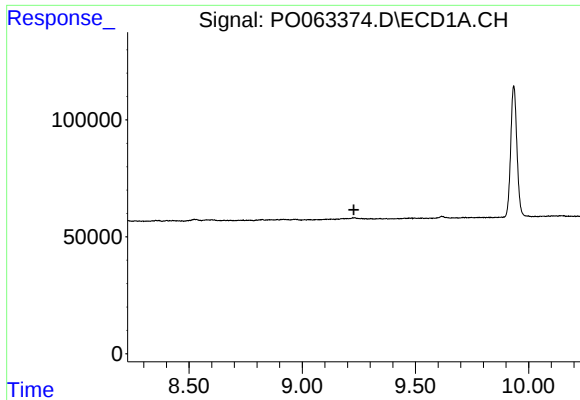

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.228 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

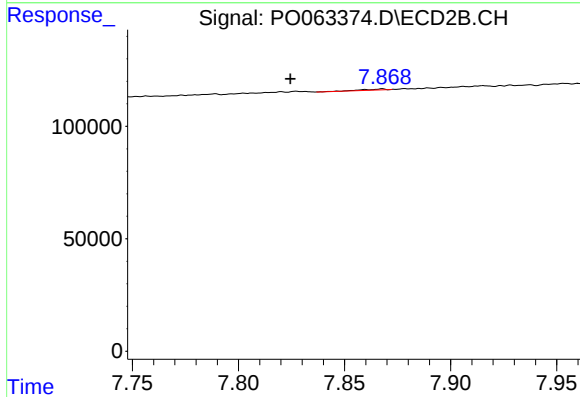


#40 AR-1262-5

R.T.: 7.868 min
Delta R.T.: 0.043 min
Response: 3189
Conc: 1.63 ng/ml

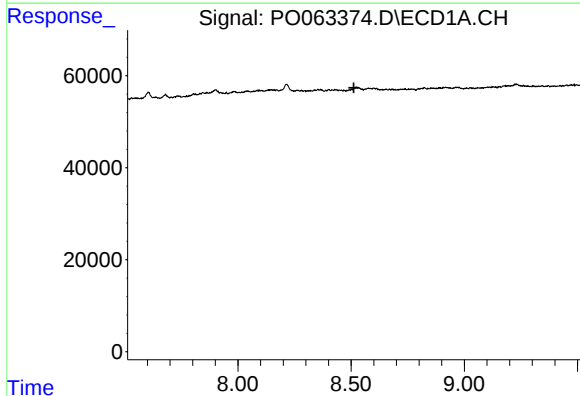


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 8.512 min
Response: 0
Conc: N.D.

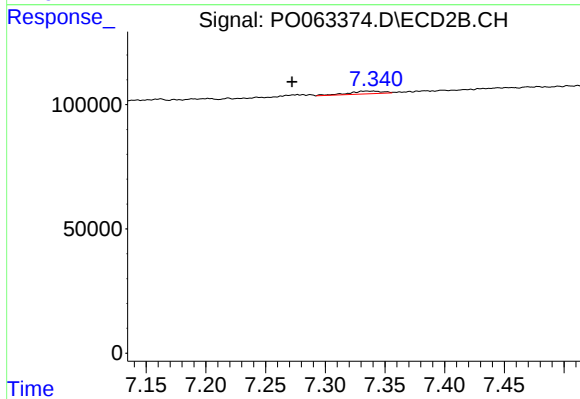

#41 AR-1268-1


R.T.: 7.335 min
Delta R.T.: 0.062 min
Response: 21275
Conc: 2.67 ng/ml

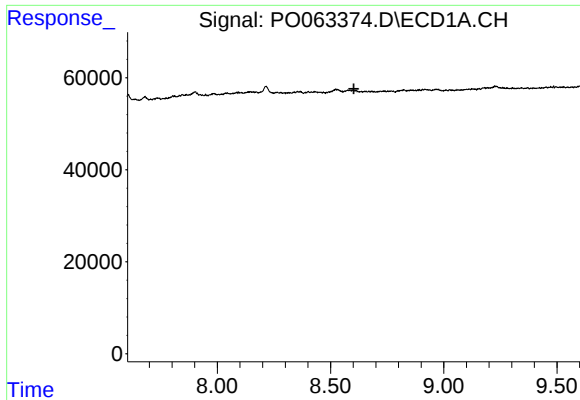

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.603 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
TP-26A-S

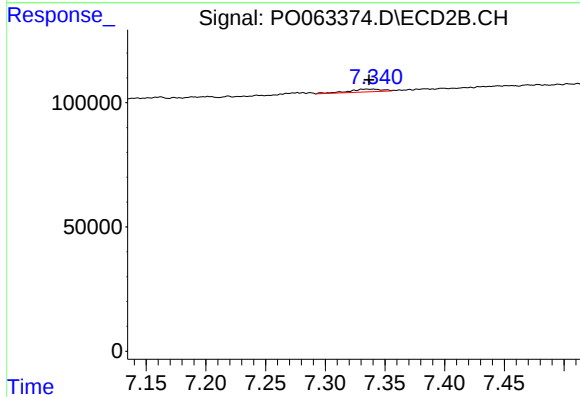


#42 AR-1268-2

R.T.: 7.335 min
Delta R.T.: -0.002 min
Response: 21275
Conc: 3.23 ng/ml

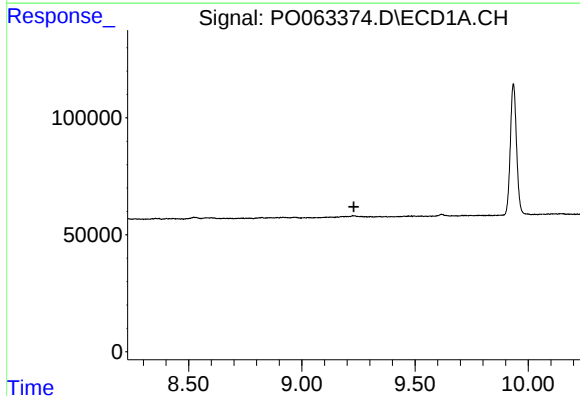

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.230 min
Response: 0
Conc: N.D.

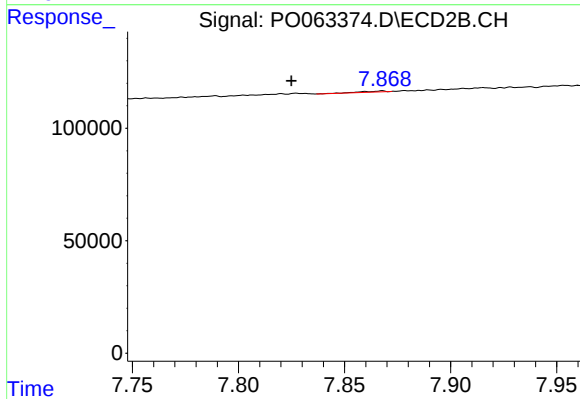

#44 AR-1268-4

R.T.: 7.868 min
Delta R.T.: 0.043 min
Response: 3189
Conc: 1.48 ng/ml