

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0103119\
 Data File : P0063355.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 31 Oct 2019 14:33
 Operator : HP/AJ
 Sample : K5147-08
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-103019

Manual Integrations
 APPROVED

Ankita
 11/1/2019 10:27:49 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 31 16:35:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.315	3.480	1315374	1426200	22.569m	26.114
2) SA Decachlor...	9.934	8.321	932812	589090	16.032	13.779

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO103119\
Data File : PO063355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 31 Oct 2019 14:33
Operator : HP/AJ
Sample : K5147-08
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OK-01-103019


Manual Integrations
APPROVED

Ankita
11/1/2019 10:27:49 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 31 16:35:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

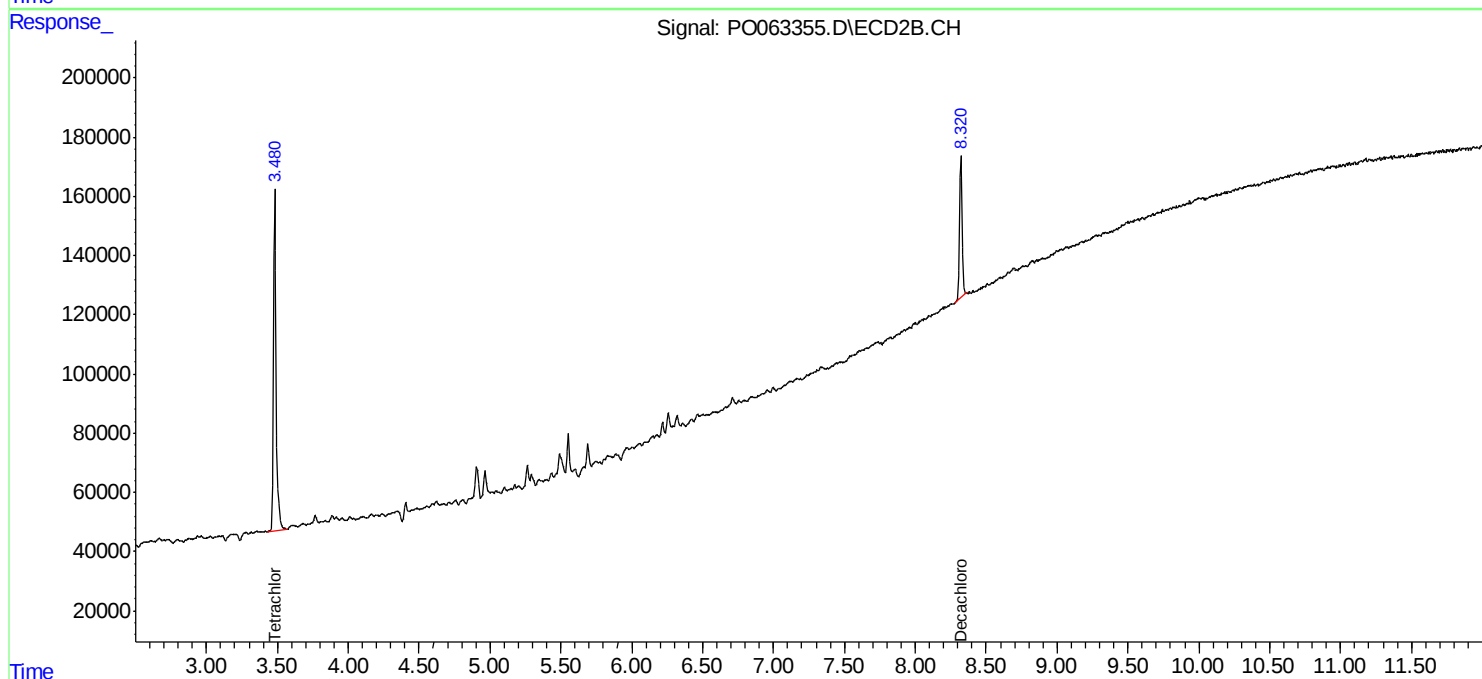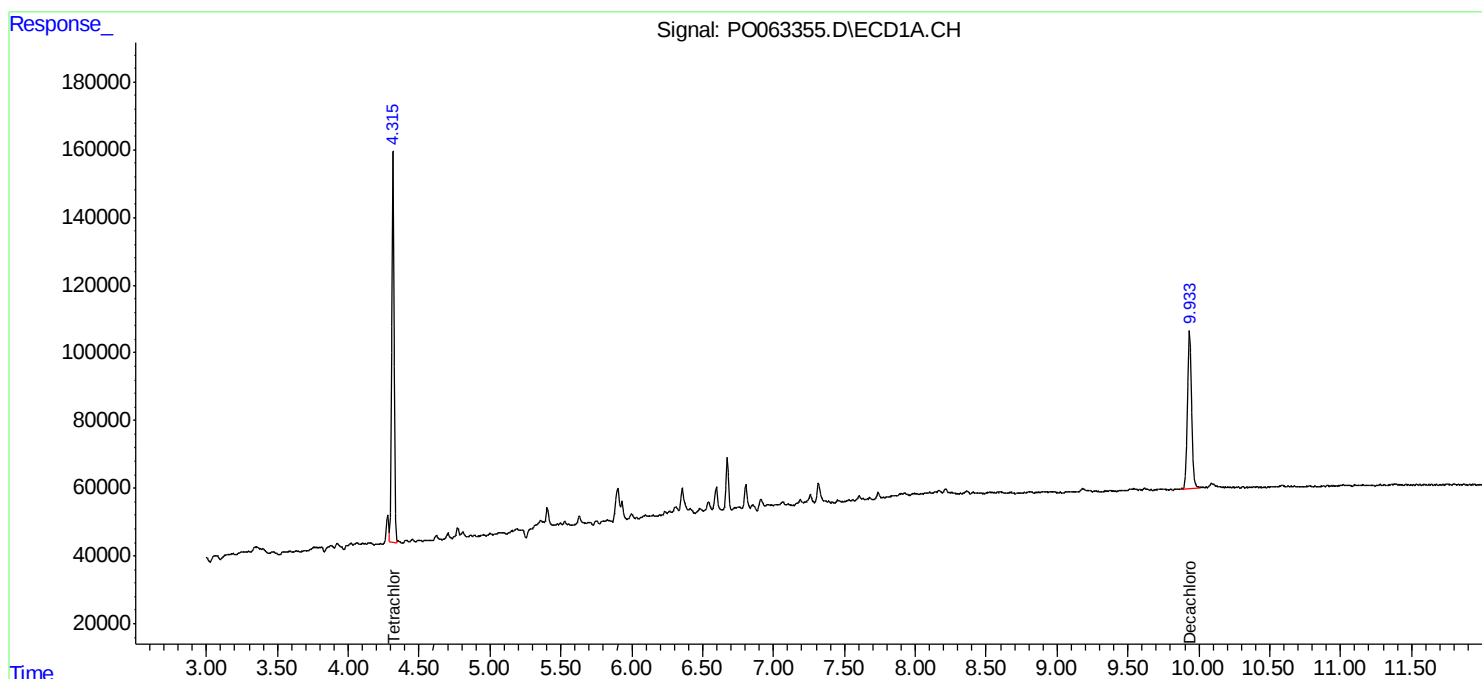

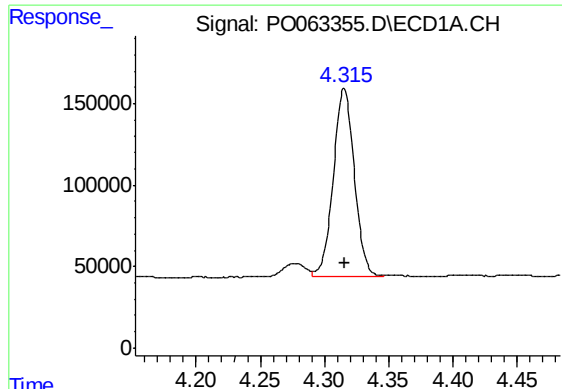


#1 Tetrachloro-m-xylene

R.T.: 4.315 min
Delta R.T.: -0.001 min
Response: 1315374
Conc: 22.57 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OK-01-103019


Manual Integrations
APPROVED

Ankita
11/1/2019 10:27:49 AM

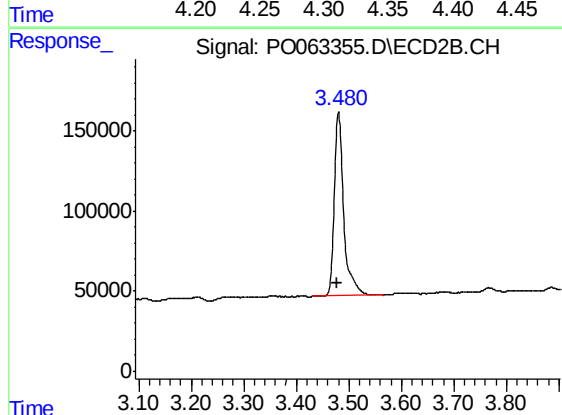


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 1426200
Conc: 26.11 ng/ml

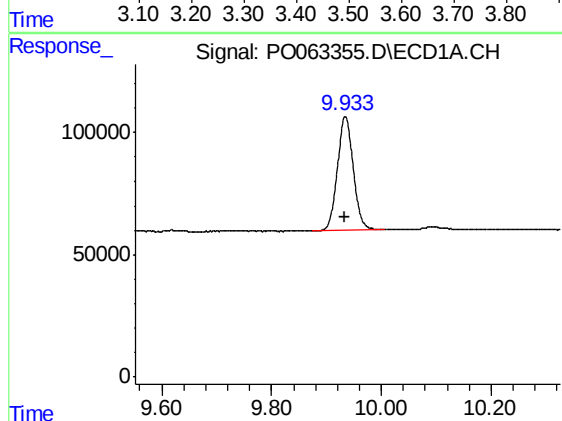

#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: 0.000 min
Response: 932812
Conc: 16.03 ng/ml

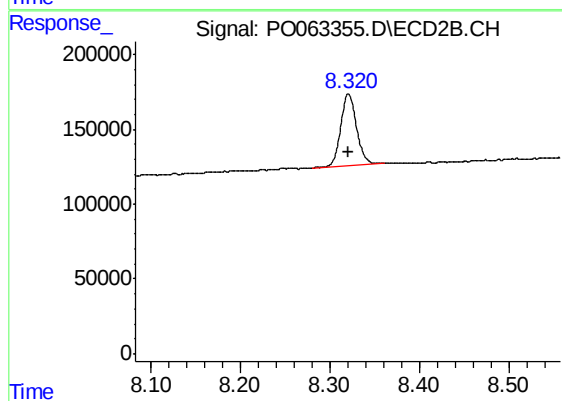

#2 Decachlorobiphenyl

R.T.: 8.321 min
Delta R.T.: 0.000 min
Response: 589090
Conc: 13.78 ng/ml