

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
 Data File : P0063396.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2019 9:08
 Operator : HP/AJ
 Sample : K5500-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 800-50-(0-2)

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:49:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 12:55:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.318	3.480	1242856	1224377	21.325	22.419
2)	SA Decachlor...	9.934	8.319	1742791	1152679	29.953	26.962
Target Compounds							
31)	L7 AR-1260-1	7.065	5.957	123599	123202	39.856	44.609
32)	L7 AR-1260-2	7.319	6.143	208218	117053	51.578	30.507 #
33)	L7 AR-1260-3	7.678	6.289	82279	76963	25.620m	24.529m
34)	L7 AR-1260-4	7.901	6.751	111214	71609	34.838m	28.283
35)	L7 AR-1260-5	8.214	6.993	121266	129506	20.677m	21.246

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
Data File : PO063396.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2019 9:08
Operator : HP/AJ
Sample : K5500-09
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
800-50-(0-2)


Manual Integrations
APPROVED

Ankita
11/4/2019 11:49:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 12:55:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

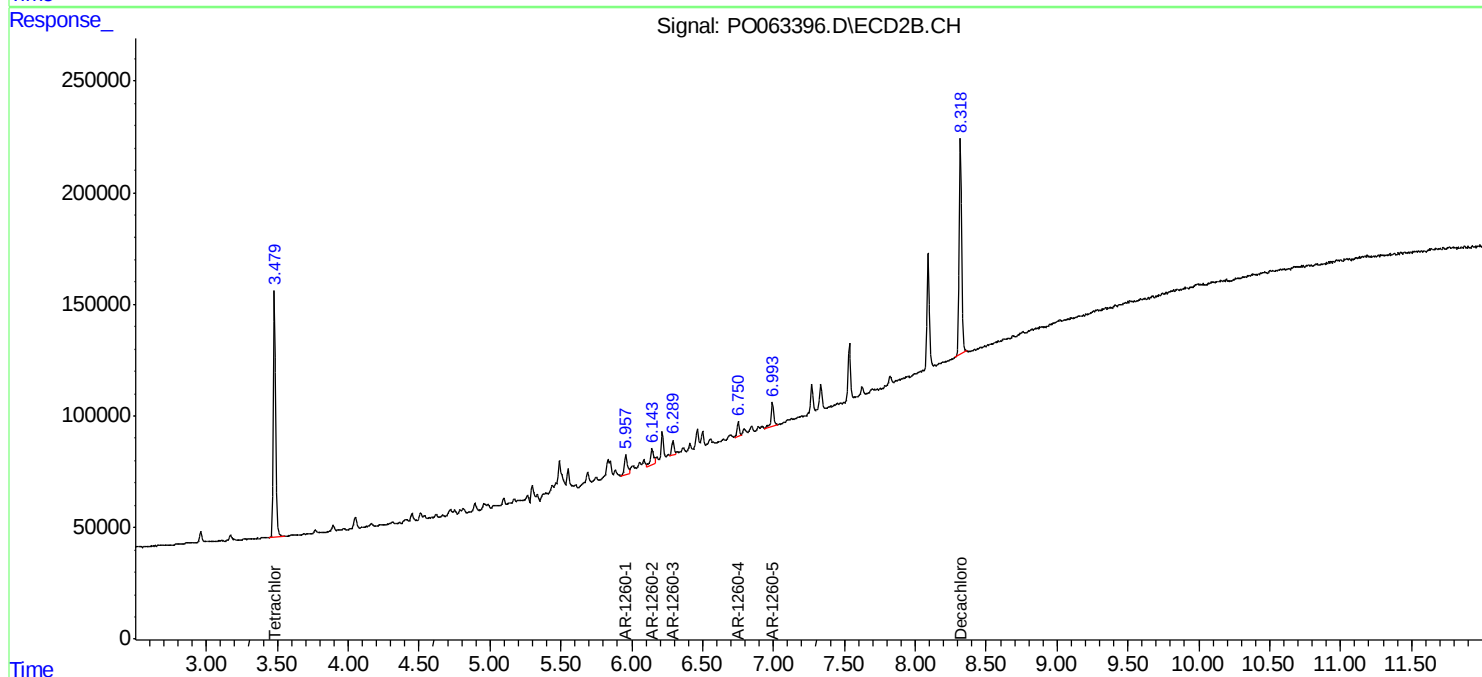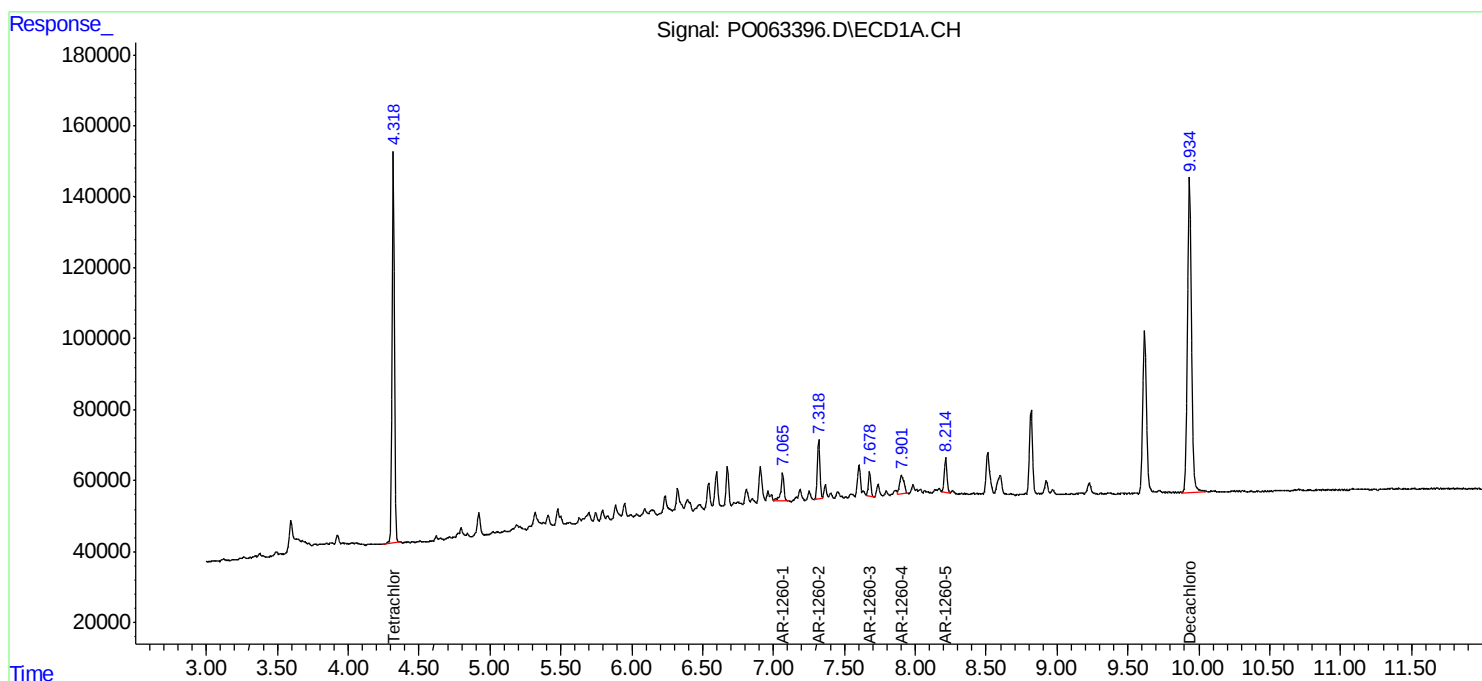

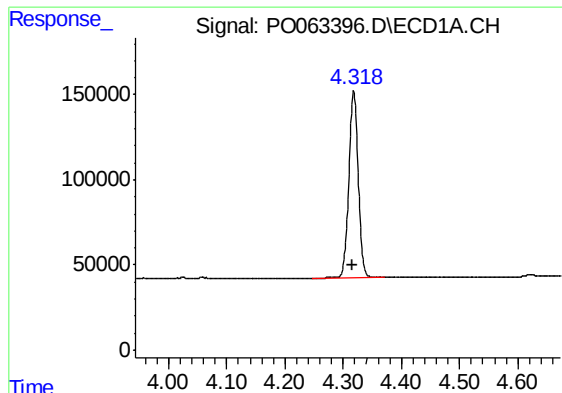


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: 0.002 min
Response: 1242856
Conc: 21.33 ng/ml

Instrument :
ECD_O
ClientSampleId :
800-50-(0-2)


Manual Integrations
APPROVED

Ankita
11/4/2019 11:49:56 AM

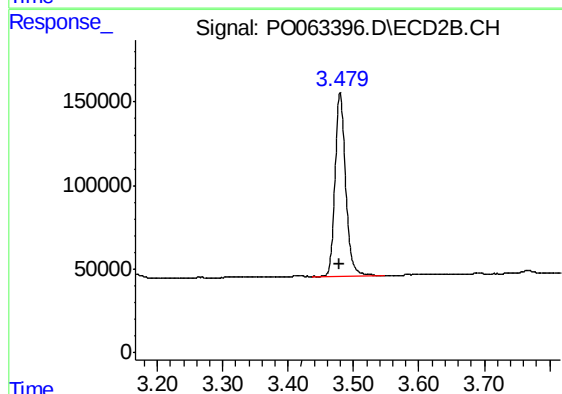


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 1224377
Conc: 22.42 ng/ml

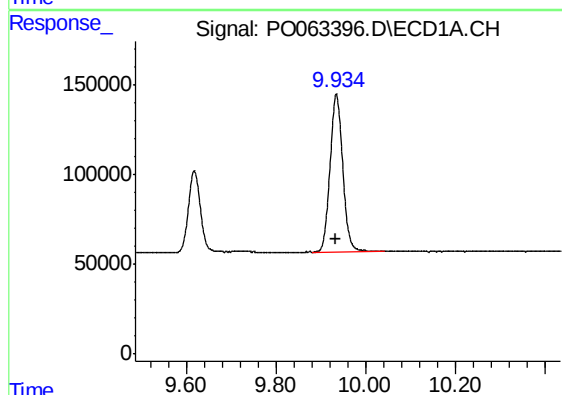


#2 Decachlorobiphenyl

R.T.: 9.934 min
Delta R.T.: 0.000 min
Response: 1742791
Conc: 29.95 ng/ml

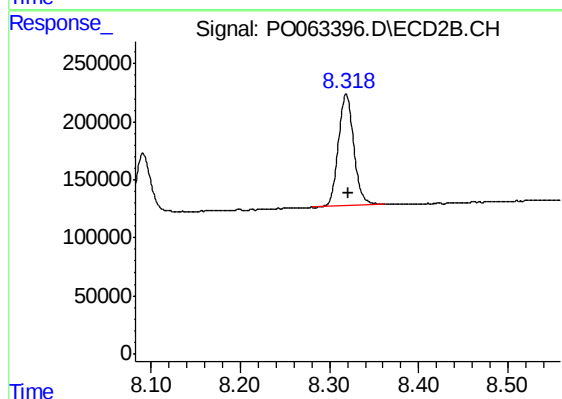

#2 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: -0.002 min
Response: 1152679
Conc: 26.96 ng/ml

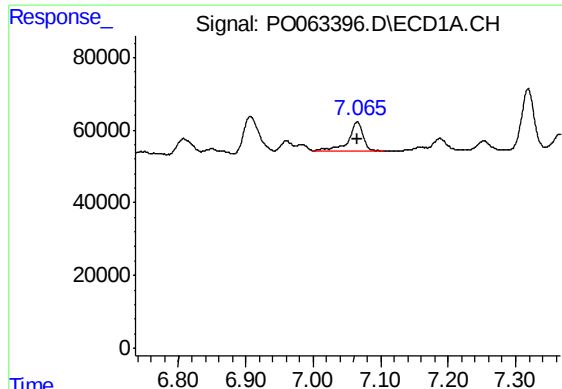


#31 AR-1260-1

R.T.: 7.065 min
Delta R.T.: 0.000 min
Response: 123599
Conc: 39.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
800-50-(0-2)


Manual Integrations
APPROVED

Ankita
11/4/2019 11:49:56 AM

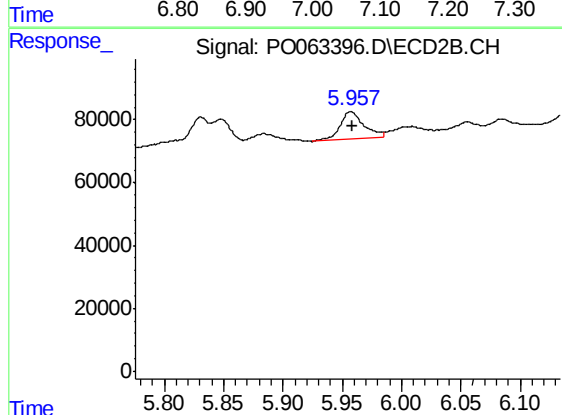


#31 AR-1260-1

R.T.: 5.957 min
Delta R.T.: -0.002 min
Response: 123202
Conc: 44.61 ng/ml

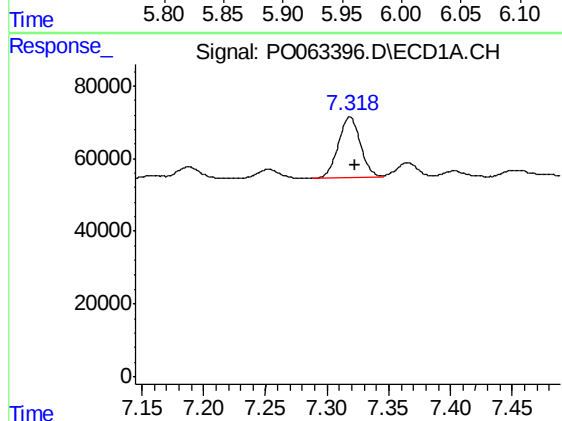


#32 AR-1260-2

R.T.: 7.319 min
Delta R.T.: -0.004 min
Response: 208218
Conc: 51.58 ng/ml

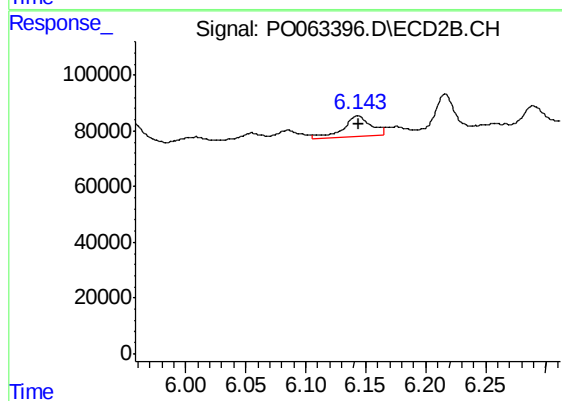

#32 AR-1260-2

R.T.: 6.143 min
Delta R.T.: -0.001 min
Response: 117053
Conc: 30.51 ng/ml

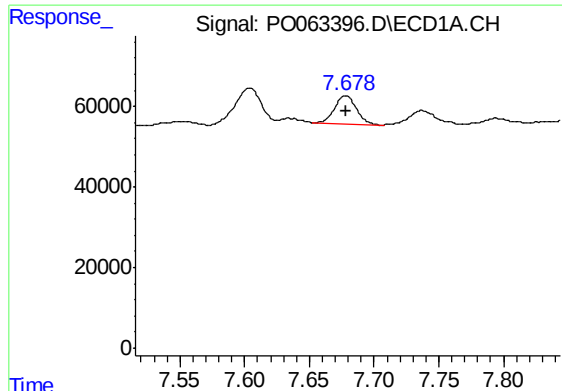


#33 AR-1260-3

R.T.: 7.678 min
Delta R.T.: 0.000 min
Response: 82279
Conc: 25.62 ng/ml m

Instrument :
ECD_O
ClientSampleId :
800-50-(0-2)


Manual Integrations
APPROVED

Ankita
11/4/2019 11:49:56 AM

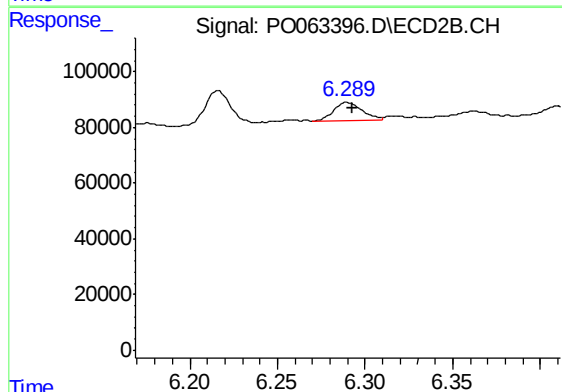


#33 AR-1260-3

R.T.: 6.289 min
Delta R.T.: -0.004 min
Response: 76963
Conc: 24.53 ng/ml m

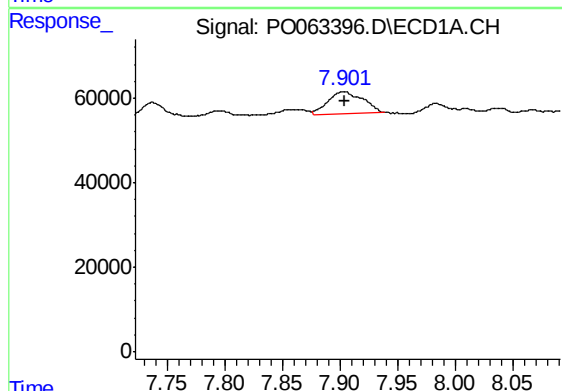


#34 AR-1260-4

R.T.: 7.901 min
Delta R.T.: -0.002 min
Response: 111214
Conc: 34.84 ng/ml m

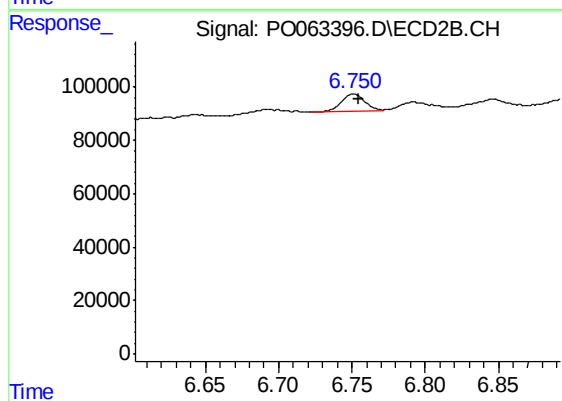

#34 AR-1260-4

R.T.: 6.751 min
Delta R.T.: -0.004 min
Response: 71609
Conc: 28.28 ng/ml

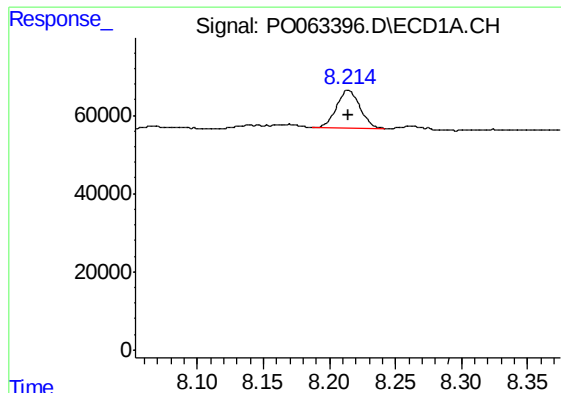


#35 AR-1260-5

R.T.: 8.214 min
Delta R.T.: 0.000 min
Response: 121266
Conc: 20.68 ng/ml m

Instrument :
ECD_O
ClientSampleId :
800-50-(0-2)

Manual Integrations
APPROVED

Ankita
11/4/2019 11:49:56 AM

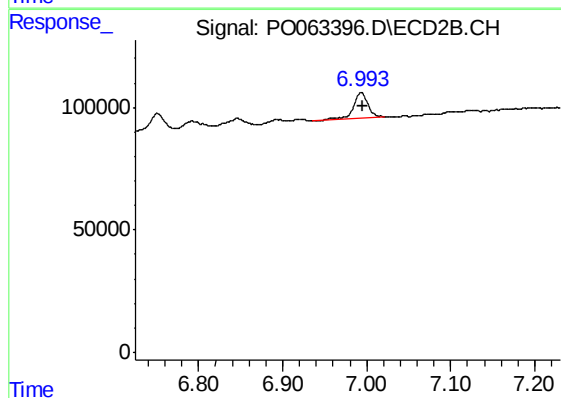

#35 AR-1260-5

R.T.: 6.993 min
Delta R.T.: -0.002 min
Response: 129506
Conc: 21.25 ng/ml