

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110119\
 Data File : P0063398.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2019 9:59
 Operator : HP/AJ
 Sample : K5625-03RE 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 03-A-03-B-03-CRE

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:50:00 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 12:56:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.318	3.481	252623	281087	4.335m	5.147
2)	SA Decachlor...	9.925	8.319	693328	664279	11.916m	15.538 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
Data File : PO063398.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2019 9:59
Operator : HP/AJ
Sample : K5625-03RE 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:00 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 12:56:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

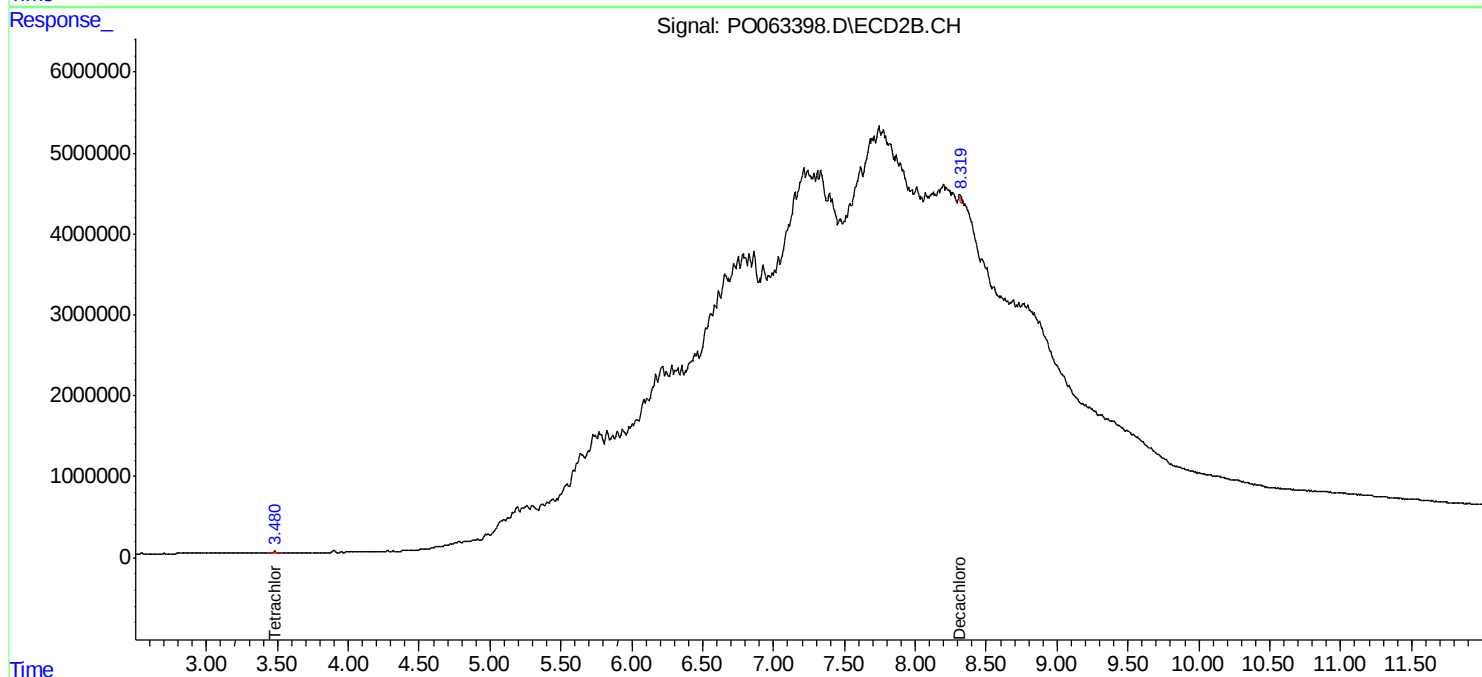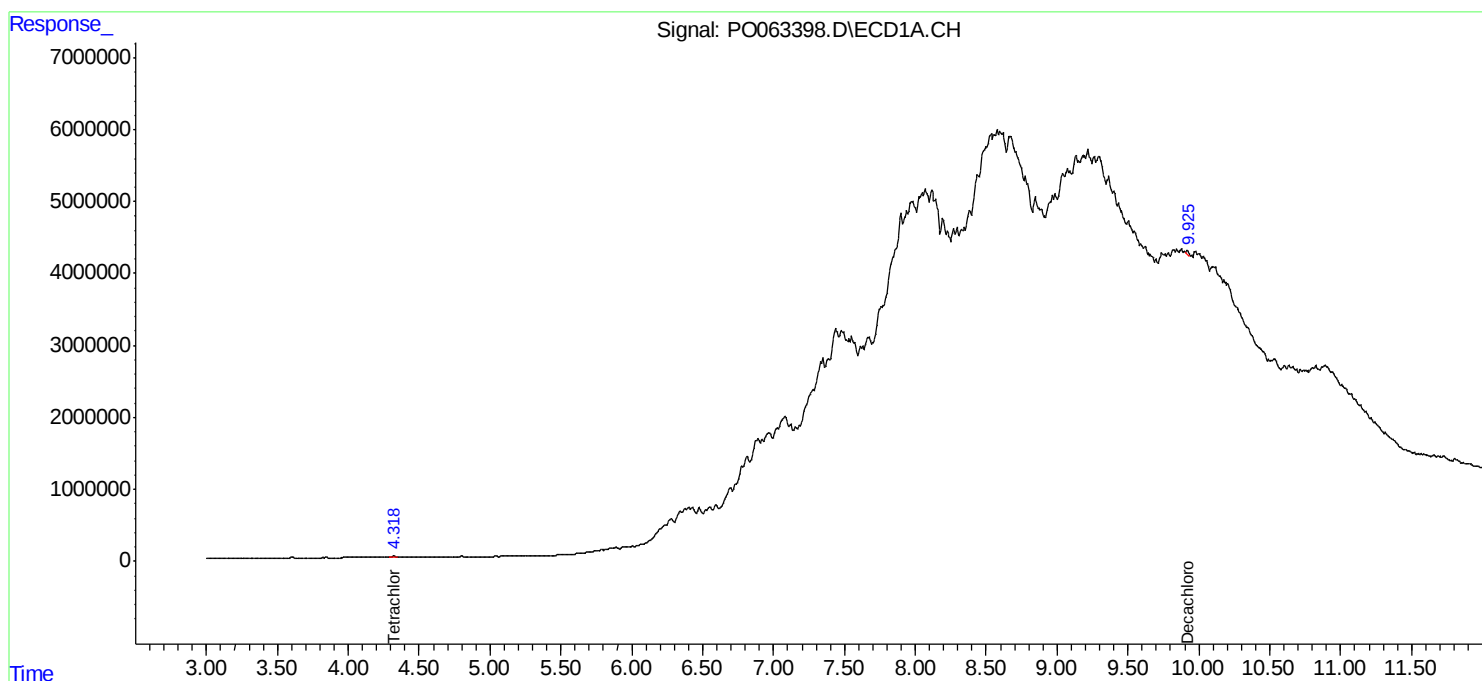

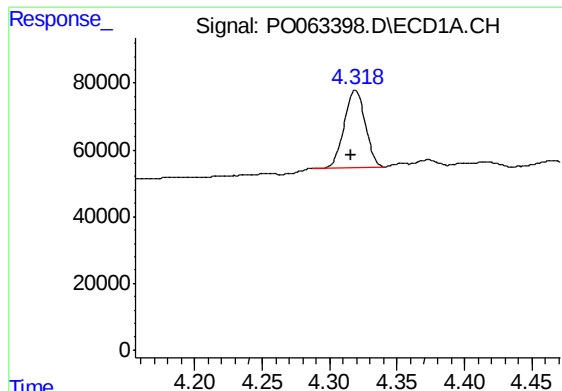


#1 Tetrachloro-m-xylene

R.T.: 4.318 min
Delta R.T.: 0.002 min
Response: 252623
Conc: 4.33 ng/ml m

Instrument :
ECD_O
ClientSampleId :
03-A-03-B-03-CRE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:00 AM

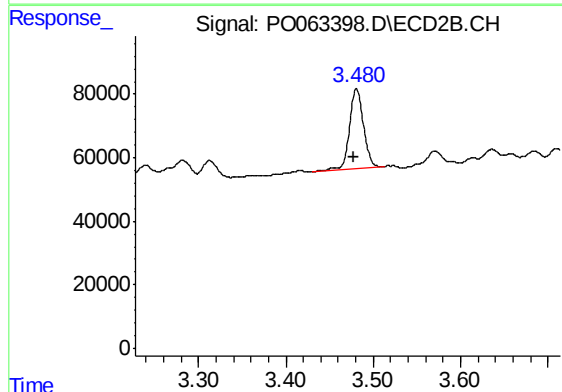


#1 Tetrachloro-m-xylene

R.T.: 3.481 min
Delta R.T.: 0.003 min
Response: 281087
Conc: 5.15 ng/ml

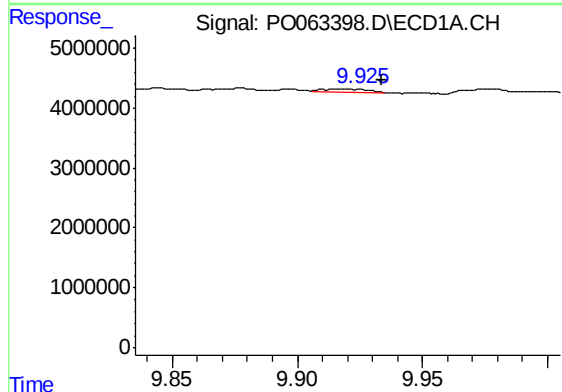

#2 Decachlorobiphenyl

R.T.: 9.925 min
Delta R.T.: -0.008 min
Response: 693328
Conc: 11.92 ng/ml m

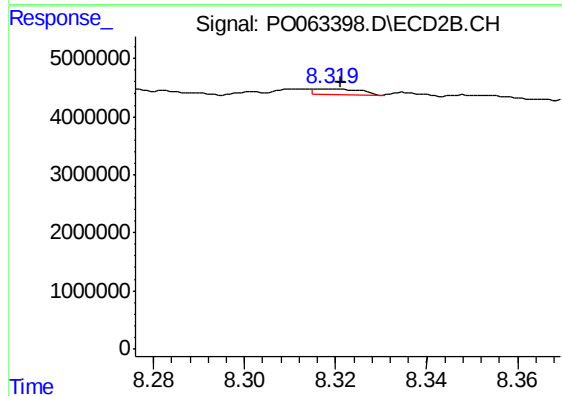

#2 Decachlorobiphenyl

R.T.: 8.319 min
Delta R.T.: -0.002 min
Response: 664279
Conc: 15.54 ng/ml