

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
 Data File : P0063401.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2019 12:34
 Operator : HP/AJ
 Sample : PB124484BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB124484BL

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:50:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 14:55:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.479	1162052	1161527	19.939m	21.268
2)	SA Decachlor...	9.926	8.315	1064005	791763	18.287m	18.520m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
Data File : PO063401.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2019 12:34
Operator : HP/AJ
Sample : PB124484BL
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PB124484BL


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 14:55:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

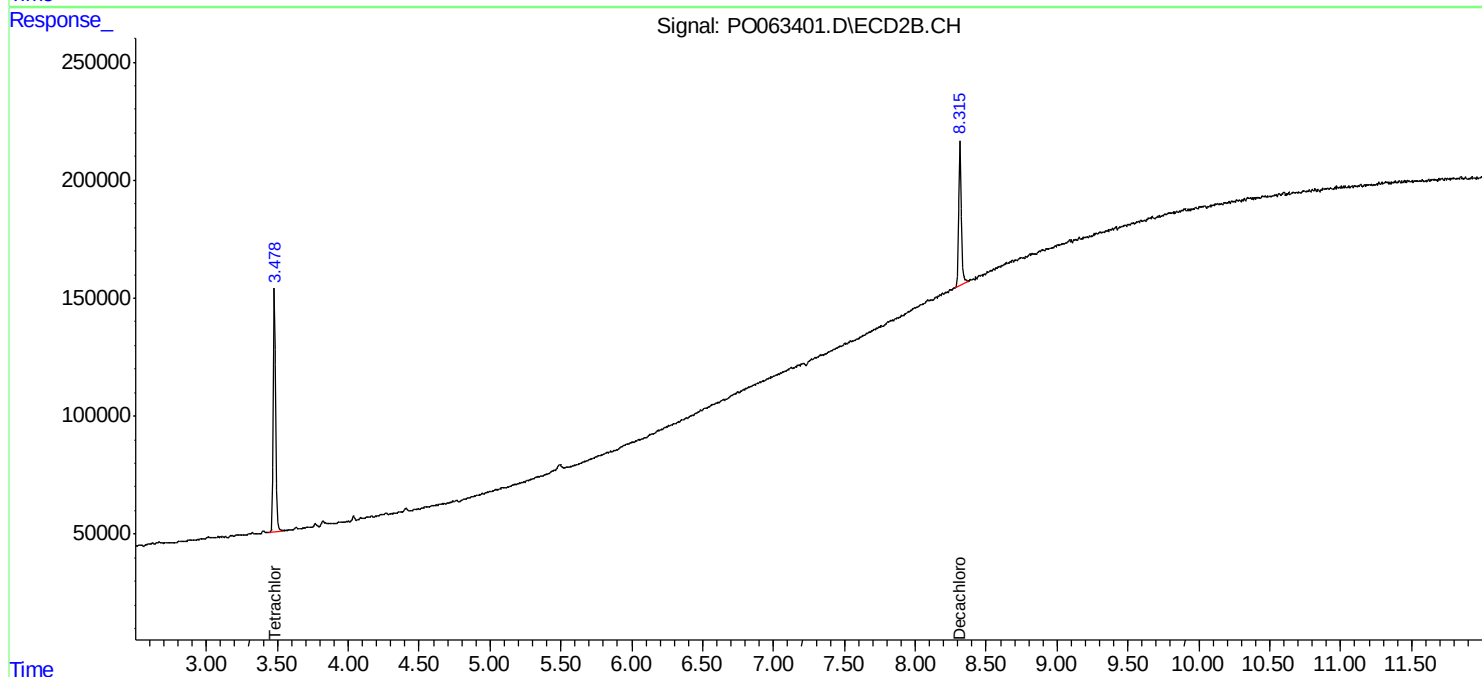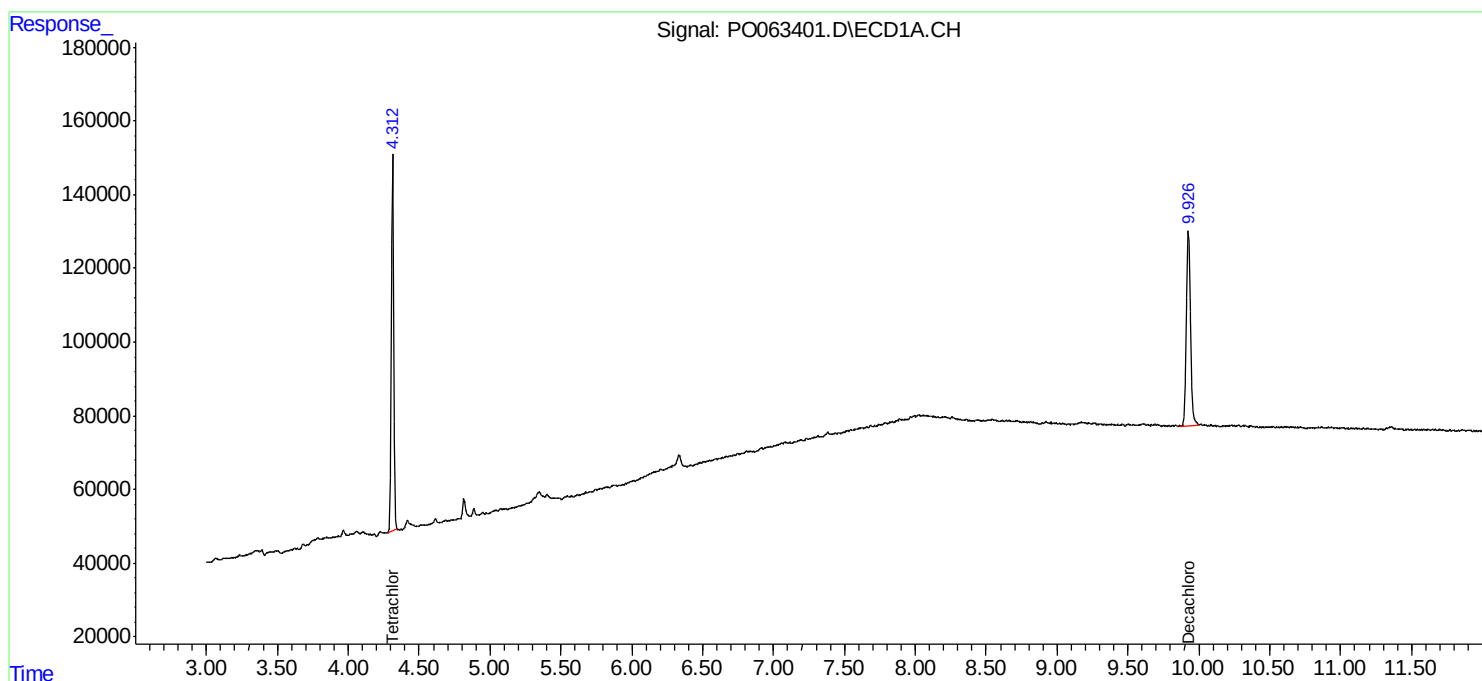

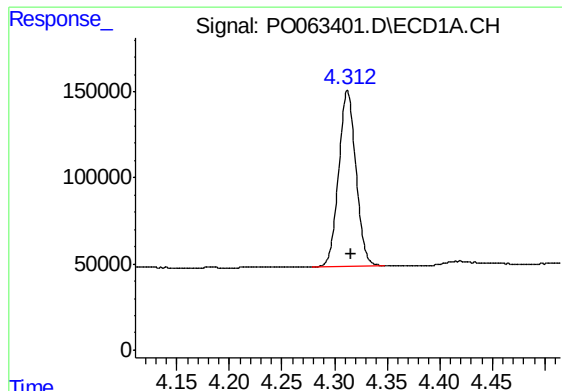


#1 Tetrachloro-m-xylene

R.T.: 4.312 min
Delta R.T.: -0.004 min
Response: 1162052
Conc: 19.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PB124484BL


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:05 AM

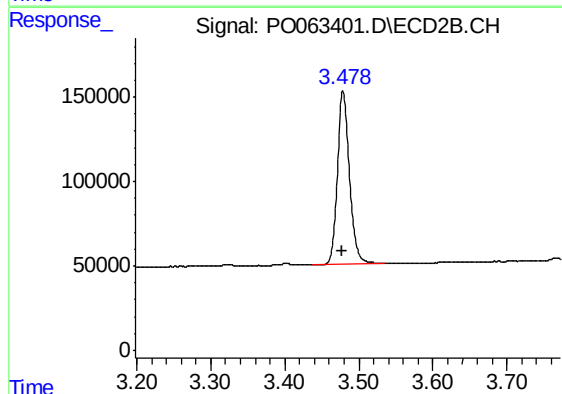


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 1161527
Conc: 21.27 ng/ml m

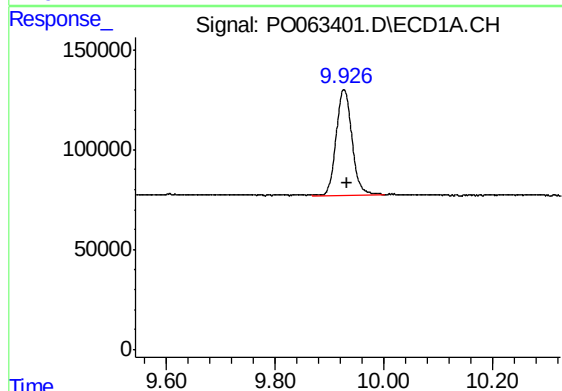

#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: -0.007 min
Response: 1064005
Conc: 18.29 ng/ml m

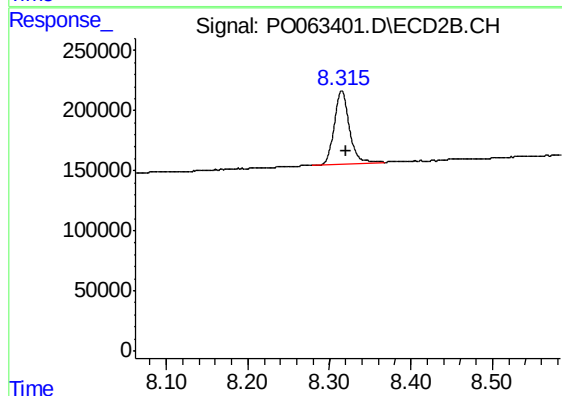

#2 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.006 min
Response: 791763
Conc: 18.52 ng/ml m