

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
 Data File : P0063408.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2019 15:11
 Operator : HP/AJ
 Sample : K5630-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-02-A

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:50:25 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 16:13:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.313	3.478	1189556	1173309	20.411m	21.484
2)	SA Decachlor...	9.924	8.316	918113	721809	15.779m	16.884
Target Compounds							
31)	L7 AR-1260-1	7.060	5.955	155563	267533	50.163m	96.867m#
32)	L7 AR-1260-2	7.312	6.140	849563	258684	210.447m	67.421m#
33)	L7 AR-1260-3	7.672	6.288	201209	183477	62.653m	58.476m
34)	L7 AR-1260-4	7.894	6.748	229895	149131	72.014m	58.901m
35)	L7 AR-1260-5	8.207	6.990	391036	332405	66.675m	54.534m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
Data File : PO063408.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2019 15:11
Operator : HP/AJ
Sample : K5630-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
S2-02-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:25 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 16:13:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

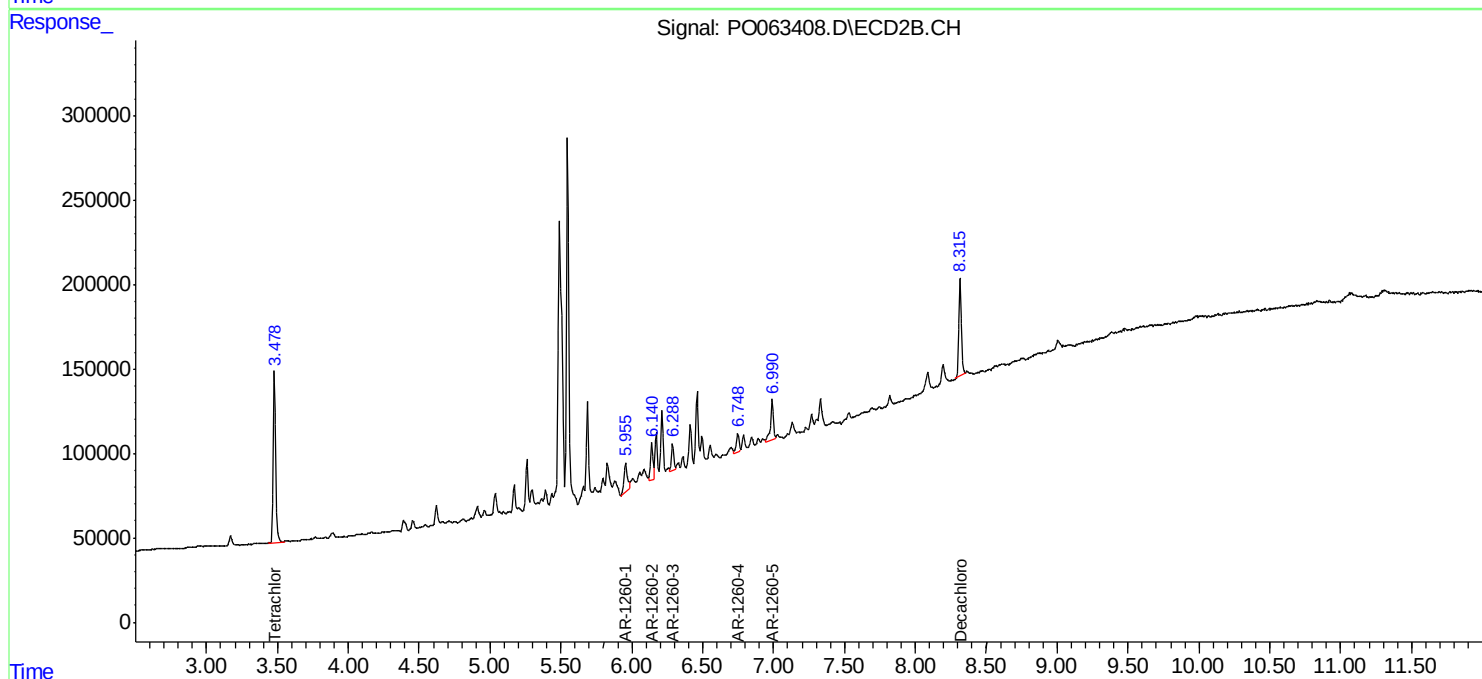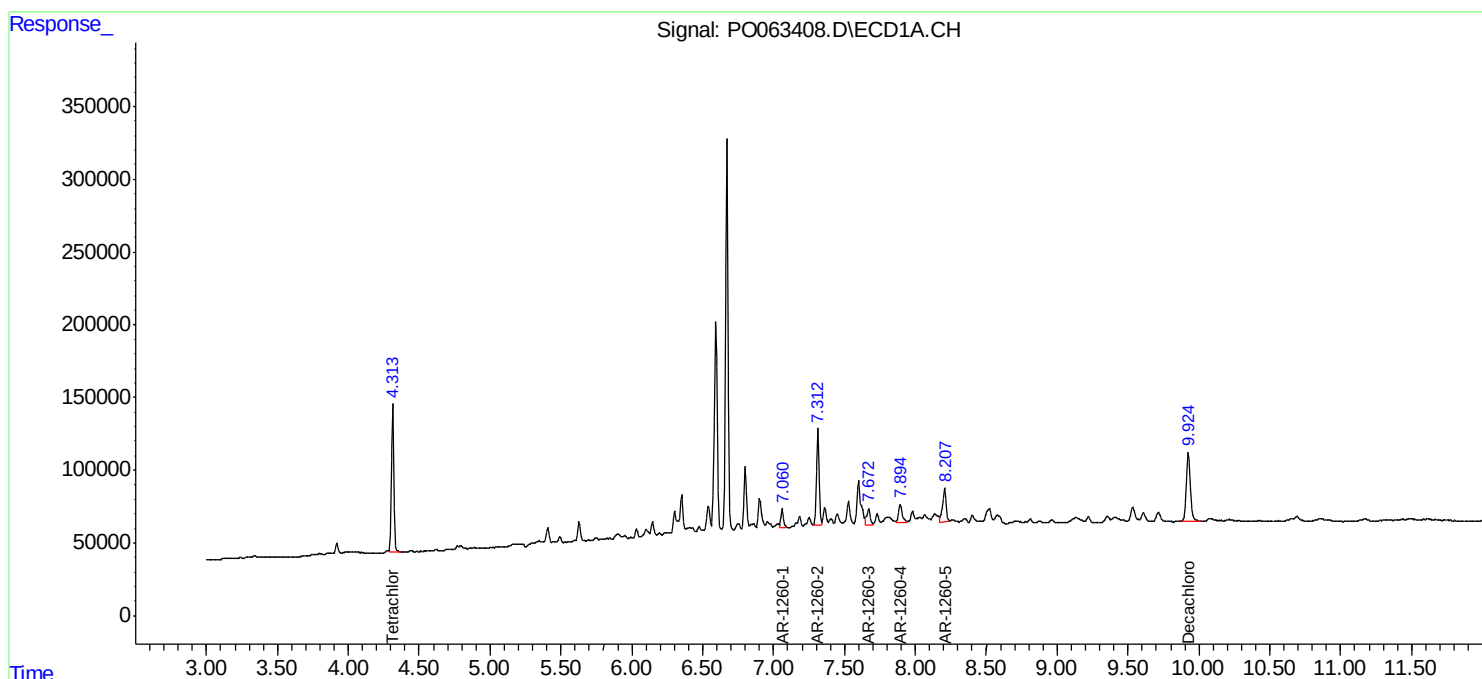

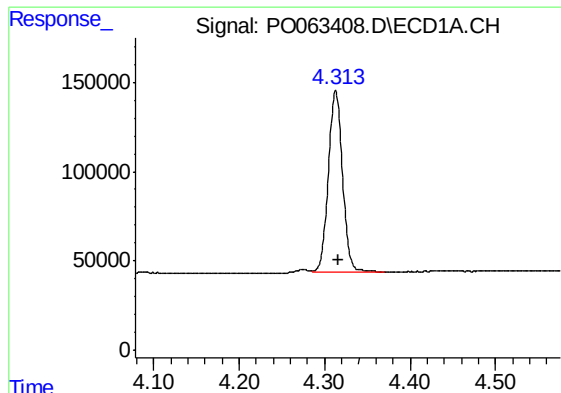


#1 Tetrachloro-m-xylene

R.T.: 4.313 min
Delta R.T.: -0.003 min
Response: 1189556
Conc: 20.41 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S2-02-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:25 AM

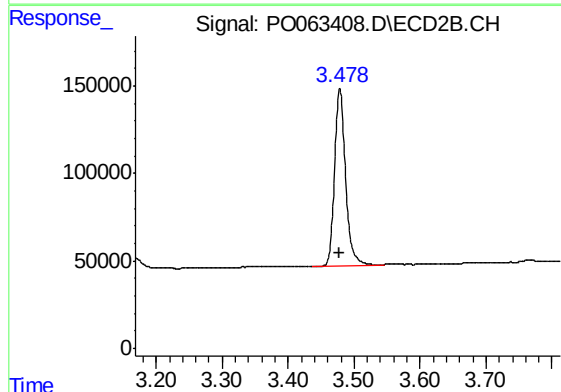


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: 0.000 min
Response: 1173309
Conc: 21.48 ng/ml

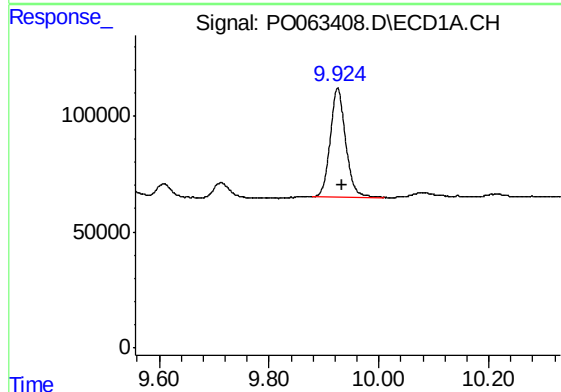


#2 Decachlorobiphenyl

R.T.: 9.924 min
Delta R.T.: -0.009 min
Response: 918113
Conc: 15.78 ng/ml m

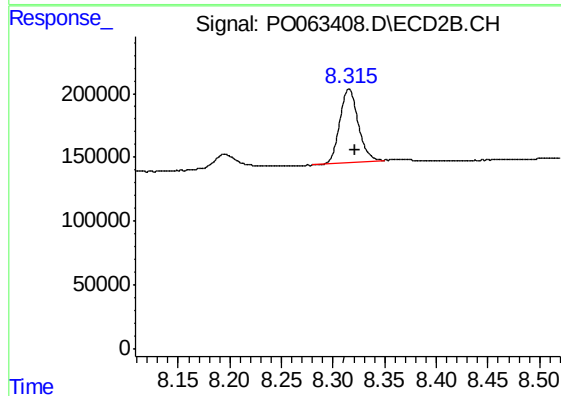

#2 Decachlorobiphenyl

R.T.: 8.316 min
Delta R.T.: -0.006 min
Response: 721809
Conc: 16.88 ng/ml

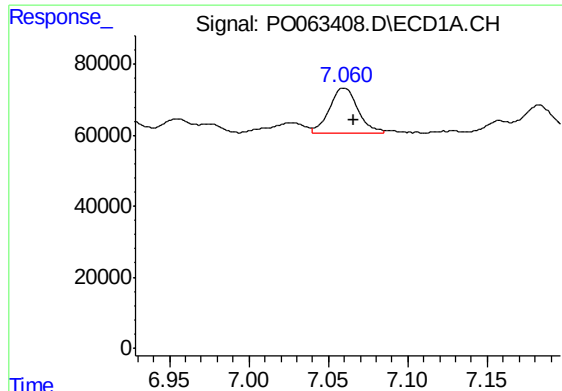


#31 AR-1260-1

R.T.: 7.060 min
Delta R.T.: -0.006 min
Response: 155563
Conc: 50.16 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S2-02-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:25 AM

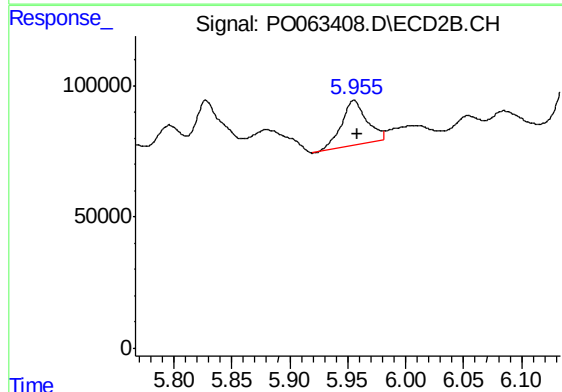


#31 AR-1260-1

R.T.: 5.955 min
Delta R.T.: -0.004 min
Response: 267533
Conc: 96.87 ng/ml m

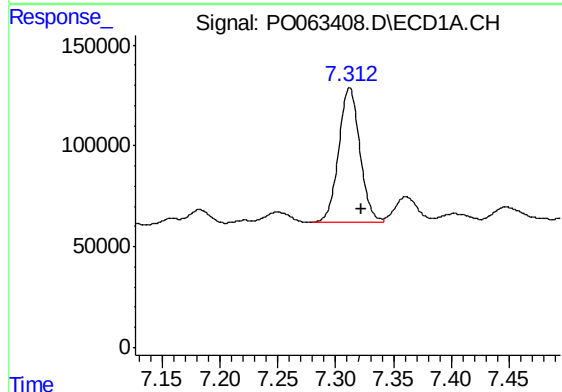


#32 AR-1260-2

R.T.: 7.312 min
Delta R.T.: -0.010 min
Response: 849563
Conc: 210.45 ng/ml m

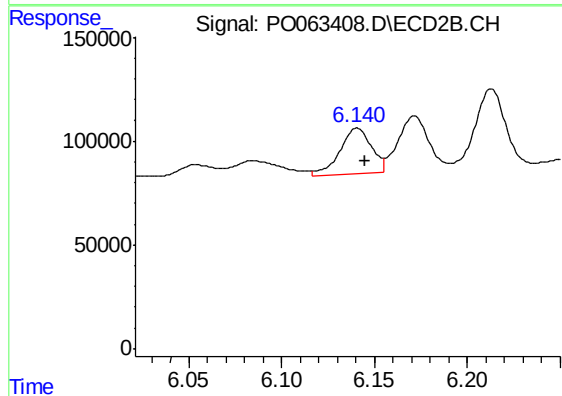

#32 AR-1260-2

R.T.: 6.140 min
Delta R.T.: -0.004 min
Response: 258684
Conc: 67.42 ng/ml m

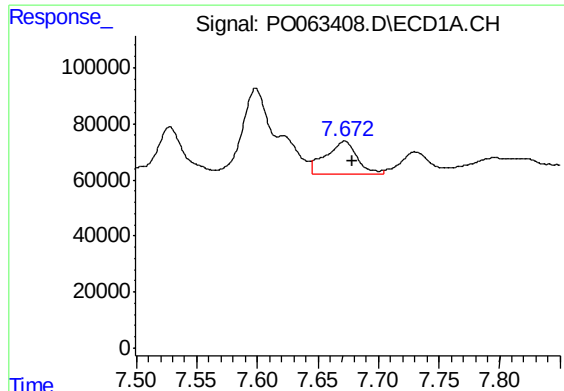


#33 AR-1260-3

R.T.: 7.672 min
Delta R.T.: -0.007 min
Response: 201209
Conc: 62.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S2-02-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:25 AM

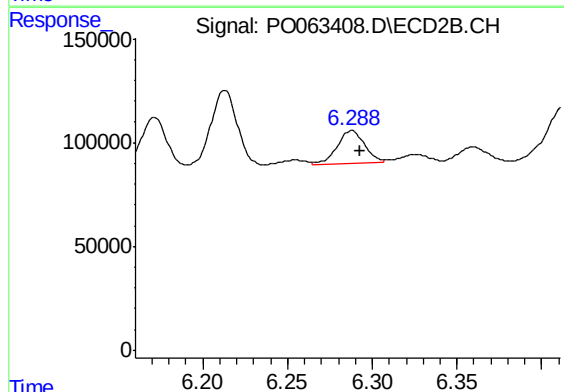


#33 AR-1260-3

R.T.: 6.288 min
Delta R.T.: -0.005 min
Response: 183477
Conc: 58.48 ng/ml m

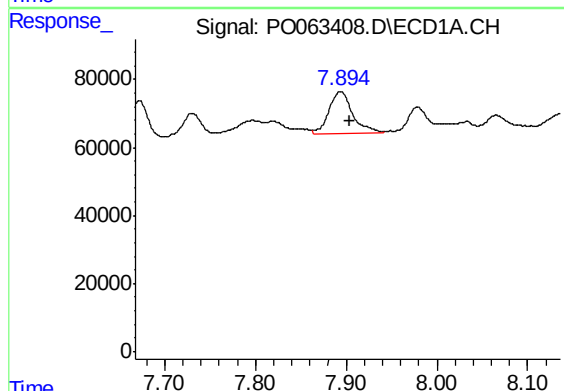


#34 AR-1260-4

R.T.: 7.894 min
Delta R.T.: -0.010 min
Response: 229895
Conc: 72.01 ng/ml m

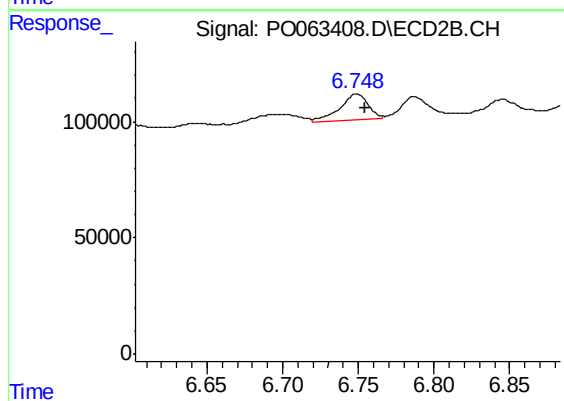

#34 AR-1260-4

R.T.: 6.748 min
Delta R.T.: -0.007 min
Response: 149131
Conc: 58.90 ng/ml m

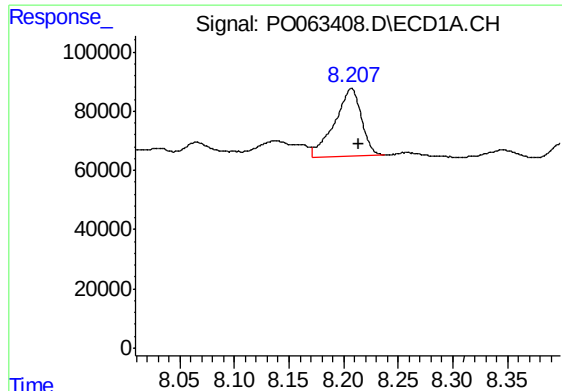


#35 AR-1260-5

R.T.: 8.207 min
Delta R.T.: -0.007 min
Response: 391036
Conc: 66.67 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S2-02-A

Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:25 AM

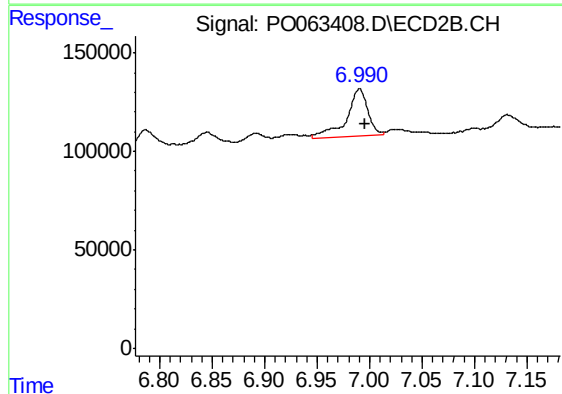

#35 AR-1260-5

R.T.: 6.990 min
Delta R.T.: -0.005 min
Response: 332405
Conc: 54.53 ng/ml m