

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
 Data File : P0063414.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Nov 2019 16:50
 Operator : HP/AJ
 Sample : K5630-22
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-4

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:50:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 01 23:23:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.479	1131023	1198358	19.406m	21.942
2)	SA Decachlor...	9.926	8.315	768800	677828	13.213	15.855
Target Compounds							
31)	L7 AR-1260-1	7.059	5.955	272713	415420	87.939m	150.414 #
32)	L7 AR-1260-2	7.313	6.140	881599	288532	218.382	75.200m#
33)	L7 AR-1260-3	7.672	6.287	268890	240042	83.728	76.504m
34)	L7 AR-1260-4	7.894	6.749	341848	183233	107.083m	72.370 #
35)	L7 AR-1260-5	8.208	6.989	477286	440838	81.381m	72.323m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
Data File : PO063414.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Nov 2019 16:50
Operator : HP/AJ
Sample : K5630-22
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
DUP-4


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 01 23:23:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

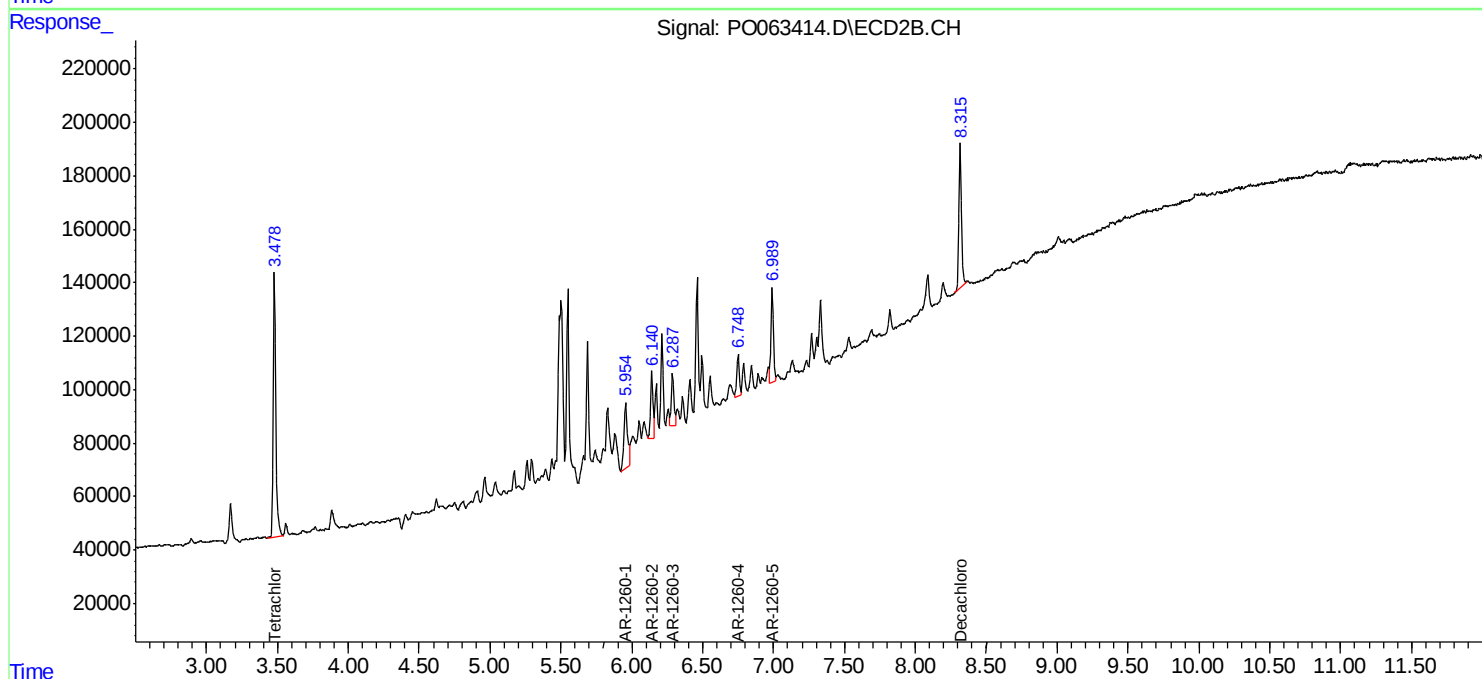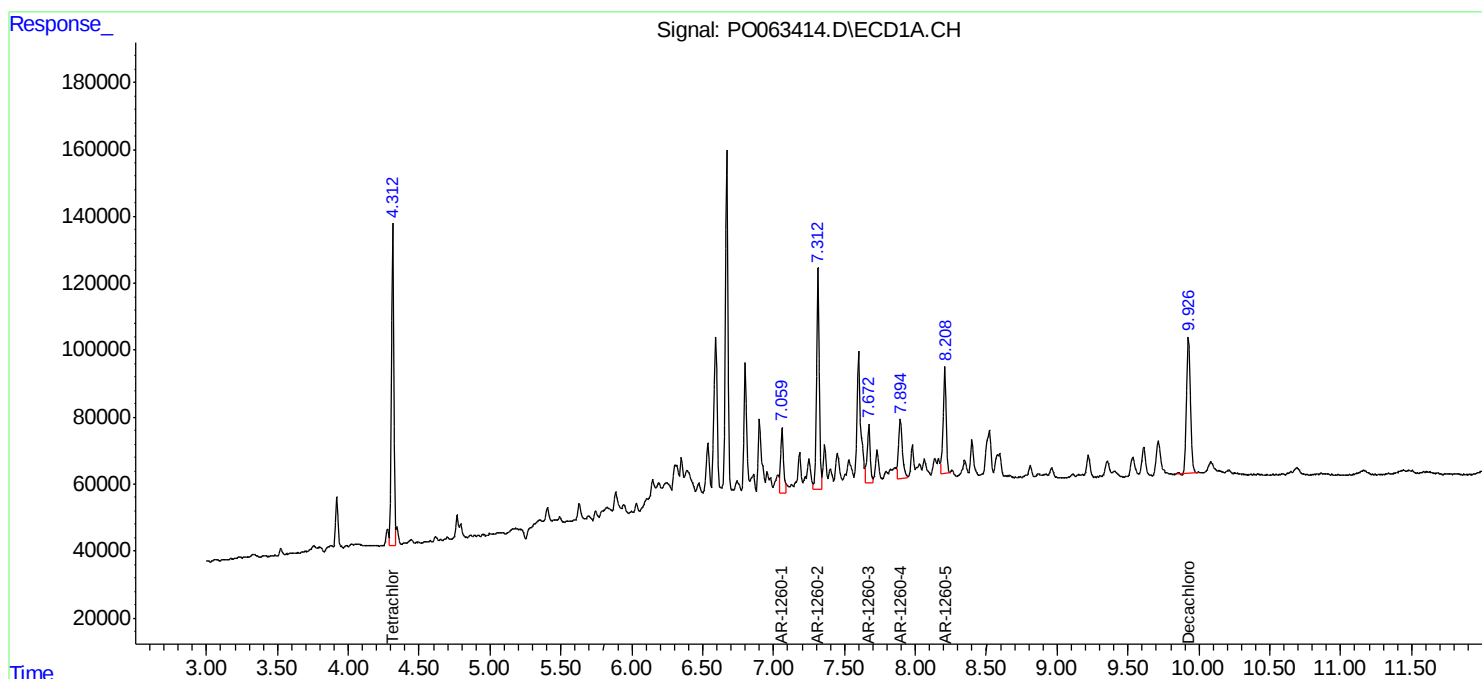

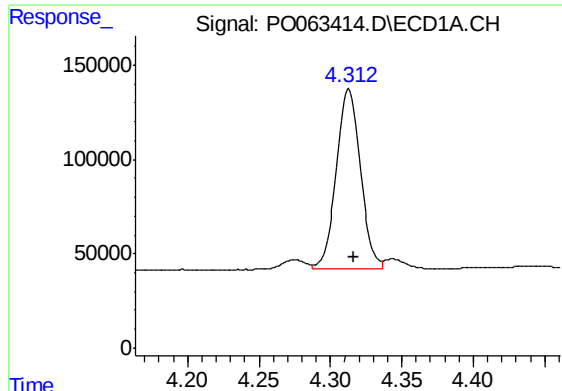


#1 Tetrachloro-m-xylene

R.T.: 4.312 min
Delta R.T.: -0.004 min
Response: 1131023
Conc: 19.41 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-4


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:54 AM

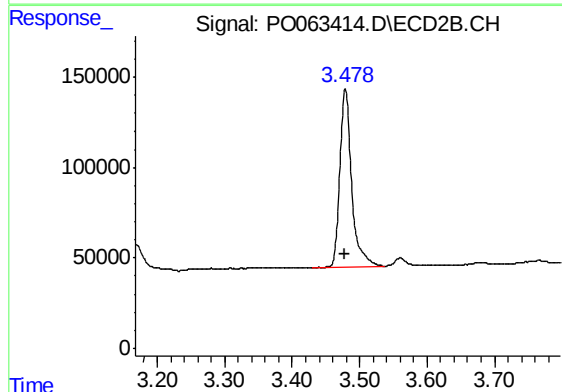


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 1198358
Conc: 21.94 ng/ml

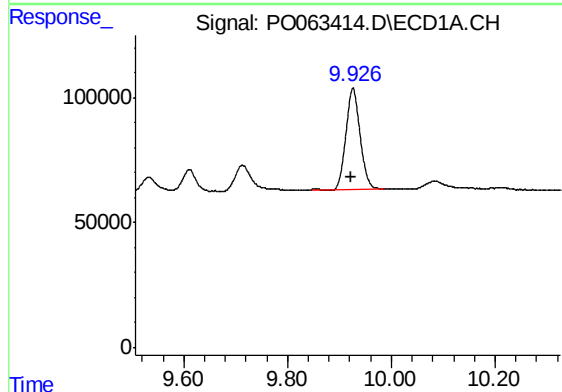


#2 Decachlorobiphenyl

R.T.: 9.926 min
Delta R.T.: 0.004 min
Response: 768800
Conc: 13.21 ng/ml

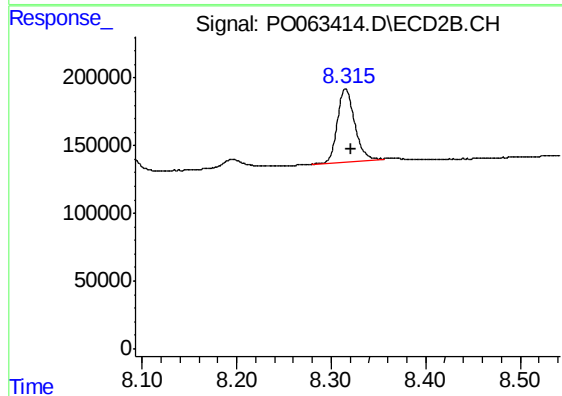

#2 Decachlorobiphenyl

R.T.: 8.315 min
Delta R.T.: -0.006 min
Response: 677828
Conc: 15.85 ng/ml

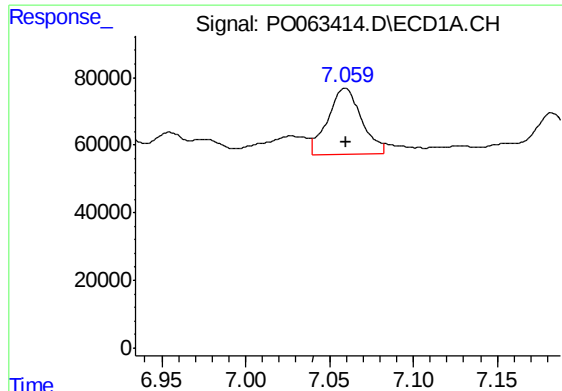


#31 AR-1260-1

R.T.: 7.059 min
Delta R.T.: 0.000 min
Response: 272713
Conc: 87.94 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-4


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:54 AM

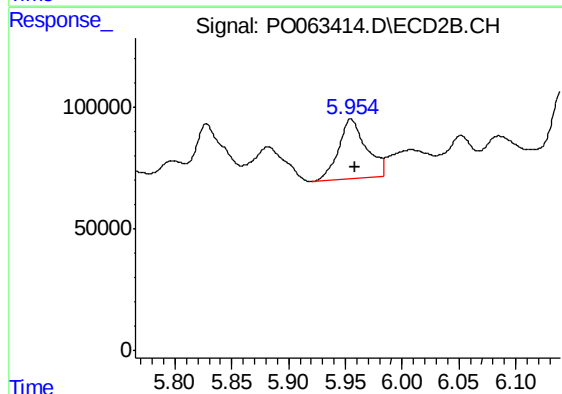


#31 AR-1260-1

R.T.: 5.955 min
Delta R.T.: -0.004 min
Response: 415420
Conc: 150.41 ng/ml

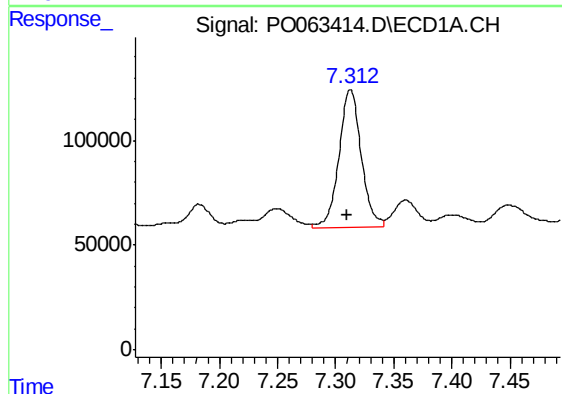


#32 AR-1260-2

R.T.: 7.313 min
Delta R.T.: 0.003 min
Response: 881599
Conc: 218.38 ng/ml

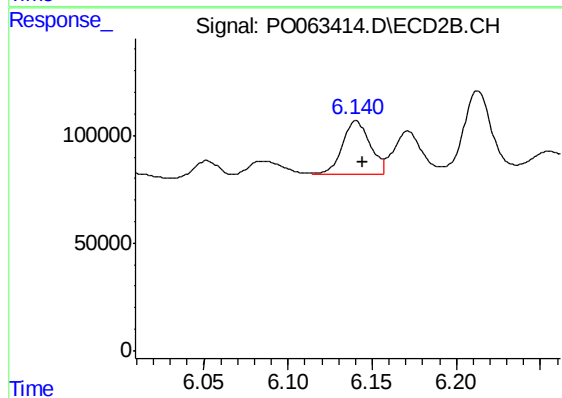

#32 AR-1260-2

R.T.: 6.140 min
Delta R.T.: -0.005 min
Response: 288532
Conc: 75.20 ng/ml m

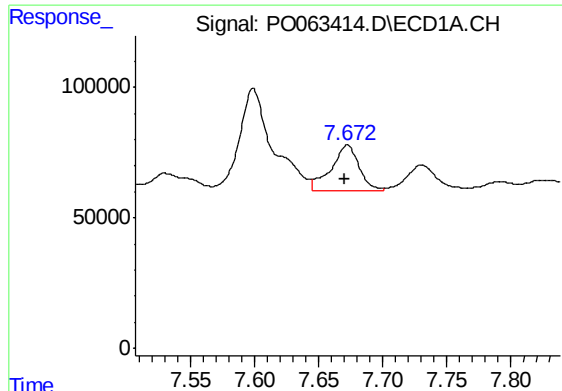


#33 AR-1260-3

R.T.: 7.672 min
Delta R.T.: 0.002 min
Response: 268890
Conc: 83.73 ng/ml

Instrument :
ECD_O
ClientSampleId :
DUP-4


Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:54 AM

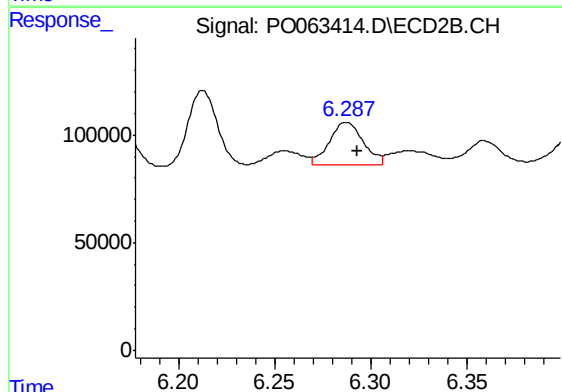


#33 AR-1260-3

R.T.: 6.287 min
Delta R.T.: -0.006 min
Response: 240042
Conc: 76.50 ng/ml m

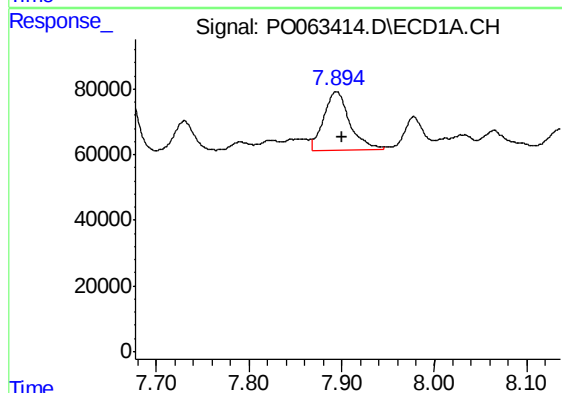


#34 AR-1260-4

R.T.: 7.894 min
Delta R.T.: -0.006 min
Response: 341848
Conc: 107.08 ng/ml m

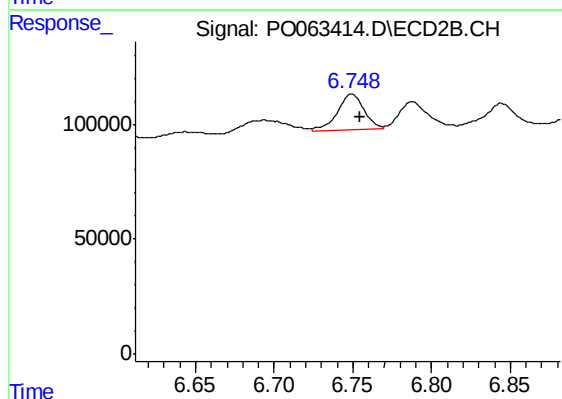

#34 AR-1260-4

R.T.: 6.749 min
Delta R.T.: -0.006 min
Response: 183233
Conc: 72.37 ng/ml

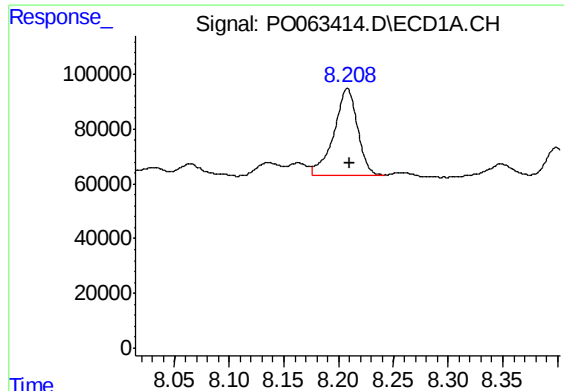


#35 AR-1260-5

R.T.: 8.208 min
Delta R.T.: -0.002 min
Response: 477286
Conc: 81.38 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-4

Manual Integrations
APPROVED

Ankita
11/4/2019 11:50:54 AM

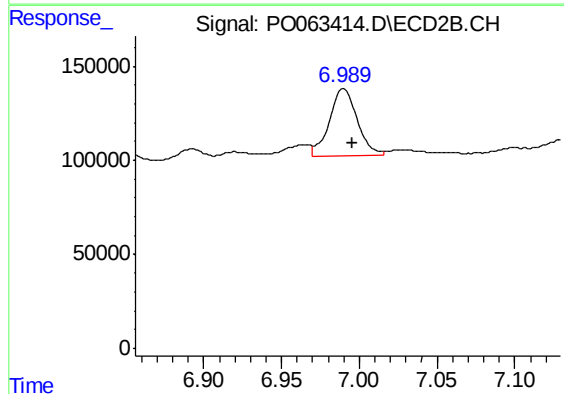

#35 AR-1260-5

R.T.: 6.989 min
Delta R.T.: -0.006 min
Response: 440838
Conc: 72.32 ng/ml m