

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110119\
Data File : P0063438.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2019 00:17
Operator : HP/AJ
Sample : K5633-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S7-08-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 00:33:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.312	3.479	738140	746803	12.665	13.674
2)	SA Decachlor...	9.922	8.312	314883	190900	5.412	4.465

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110119\
Data File : PO063438.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2019 00:17
Operator : HP/AJ
Sample : K5633-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S7-08-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 02 00:33:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

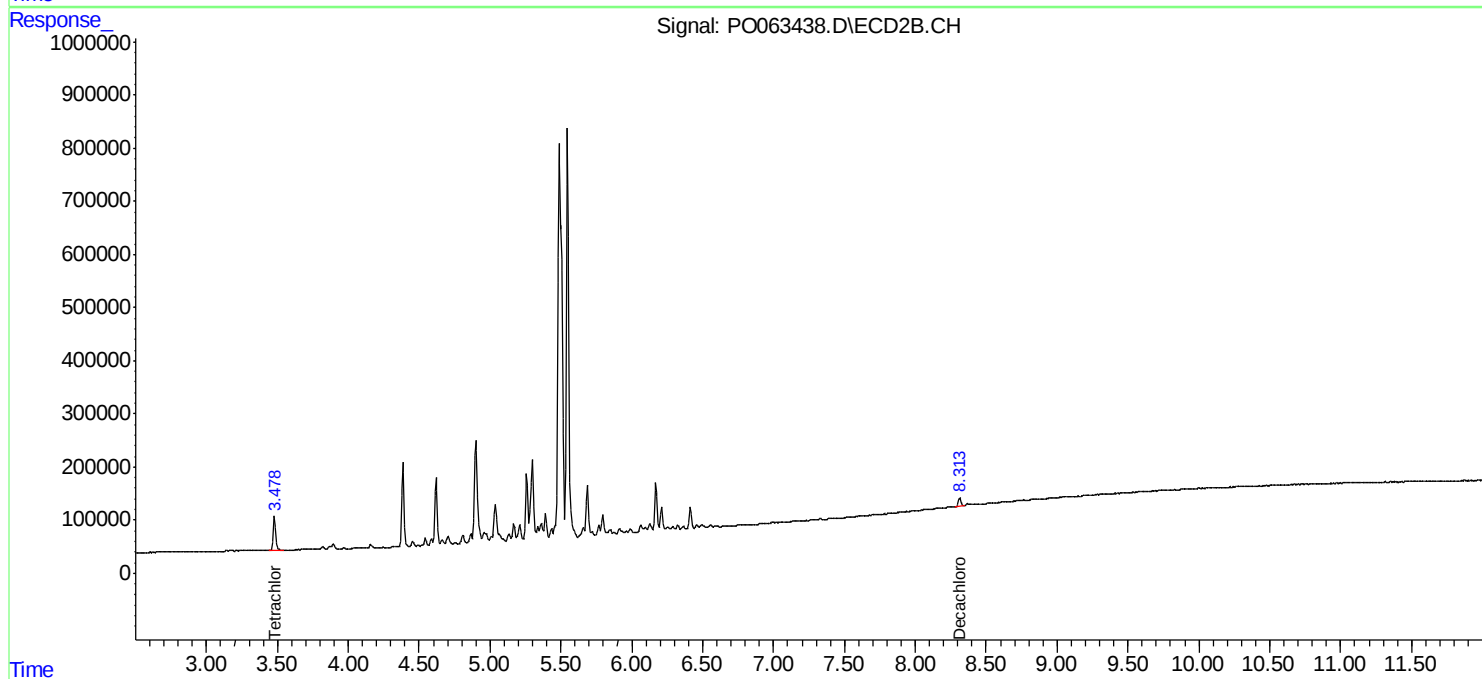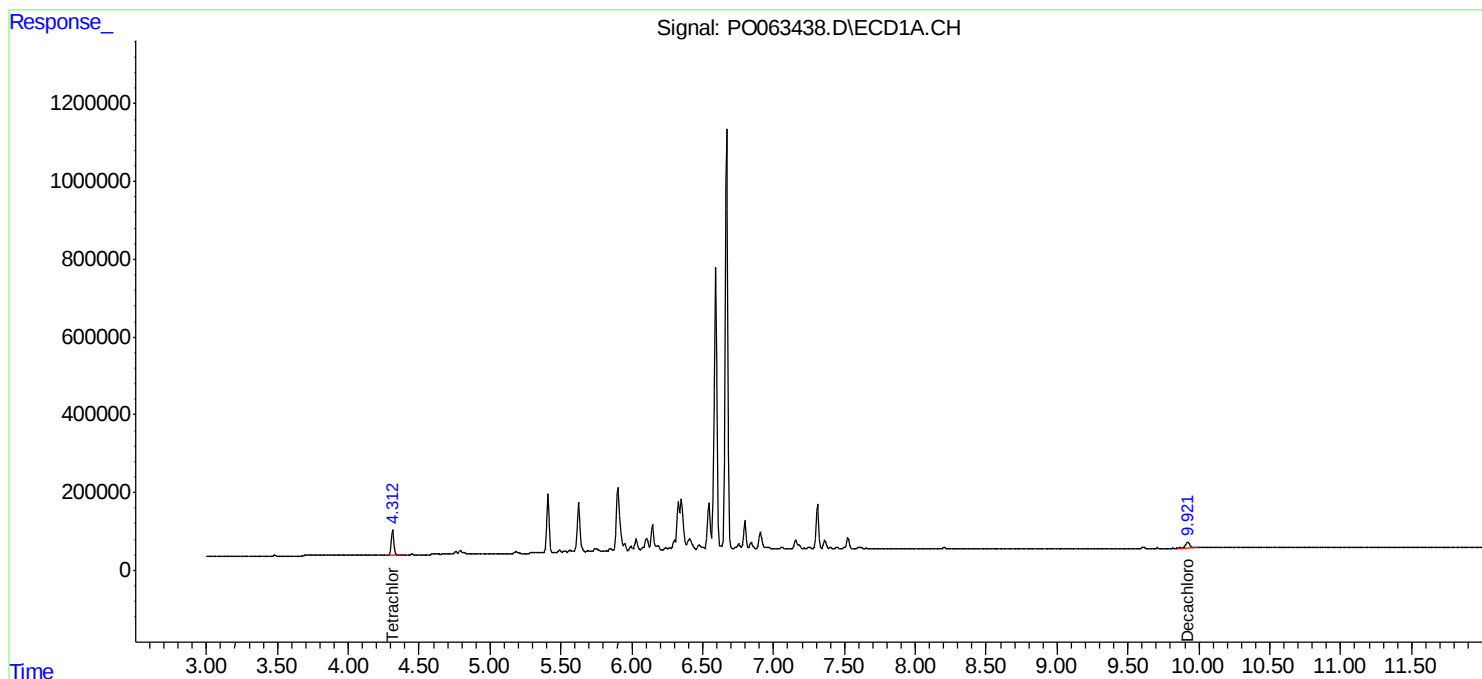


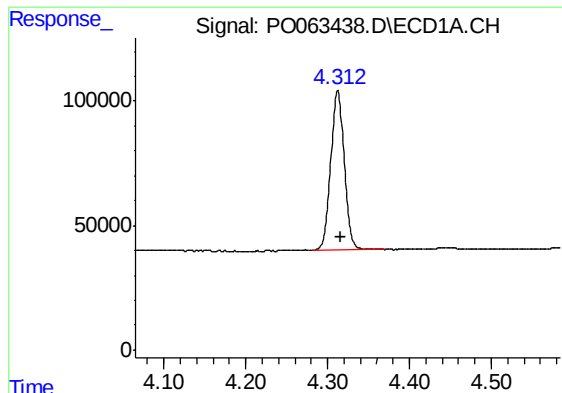

#1 Tetrachloro-m-xylene


R.T.: 4.312 min
Delta R.T.: -0.004 min
Response: 738140
Conc: 12.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-08-A

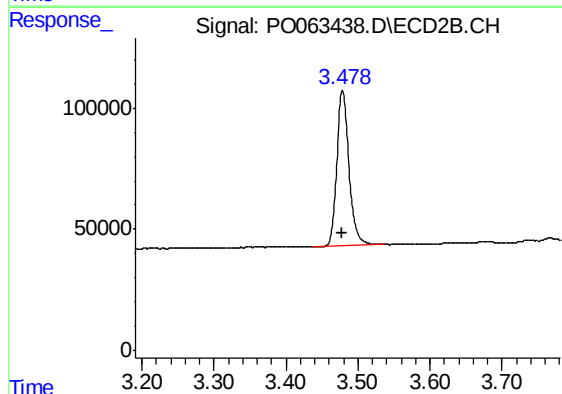


#1 Tetrachloro-m-xylene

R.T.: 3.479 min
Delta R.T.: 0.000 min
Response: 746803
Conc: 13.67 ng/ml

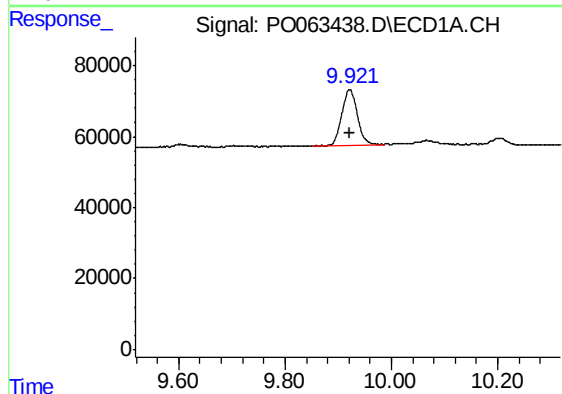

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: 0.000 min
Response: 314883
Conc: 5.41 ng/ml

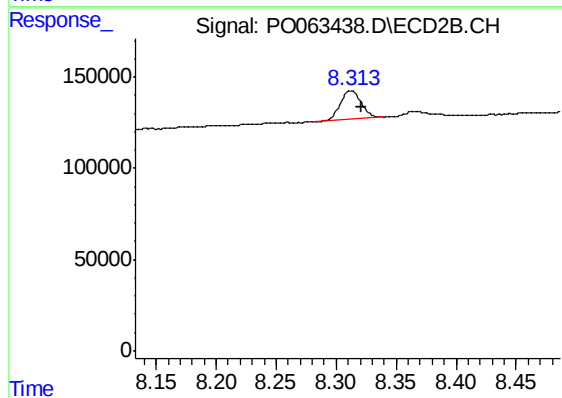

#2 Decachlorobiphenyl

R.T.: 8.312 min
Delta R.T.: -0.009 min
Response: 190900
Conc: 4.47 ng/ml