

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110219\
 Data File : P0063457.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2019 10:05
 Operator : HP/AJ
 Sample : K5632-04RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S3-04-ARE

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:53:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:27:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.311	3.478	862888	892679	14.806m	16.345
2) SA Decachlor...	9.920	8.312	494772	326943	8.503	7.647

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
Data File : PO063457.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2019 10:05
Operator : HP/AJ
Sample : K5632-04RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S3-04-ARE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:53:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:27:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

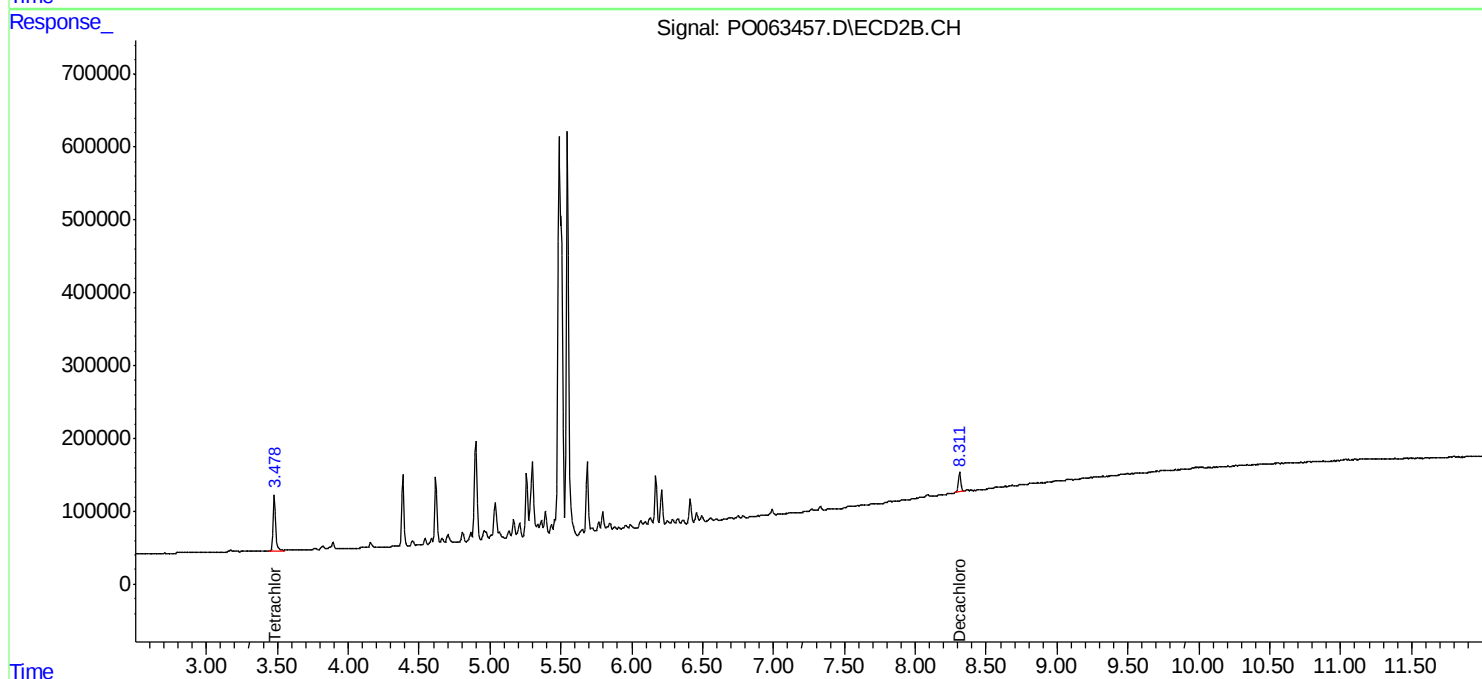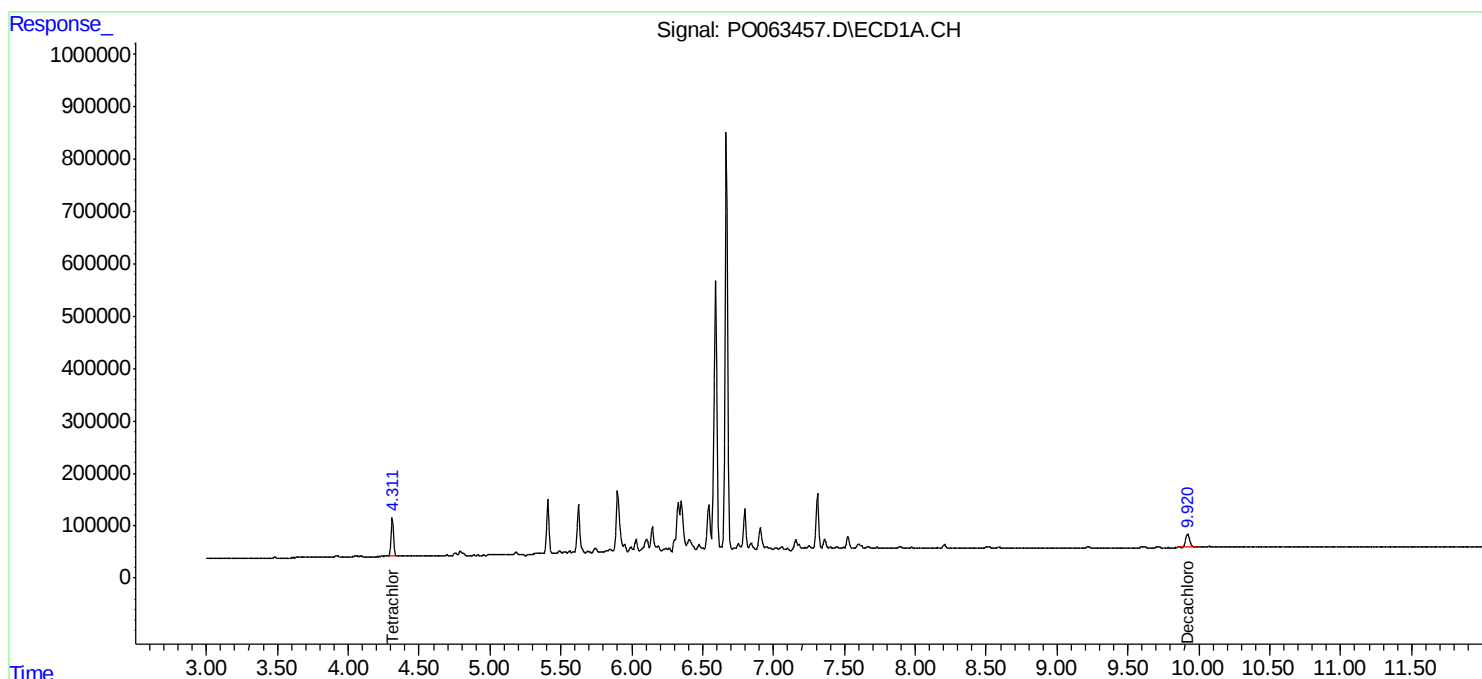

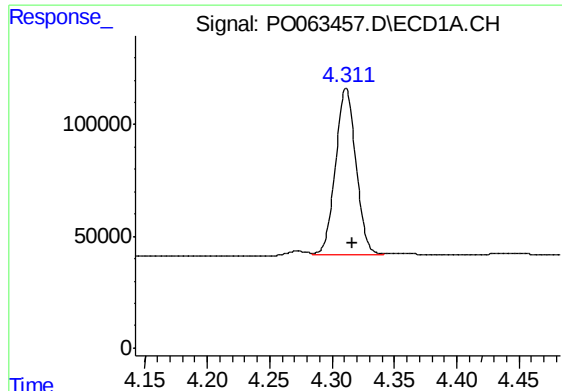


#1 Tetrachloro-m-xylene

R.T.: 4.311 min
Delta R.T.: -0.005 min
Response: 862888
Conc: 14.81 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S3-04-ARE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:53:40 AM

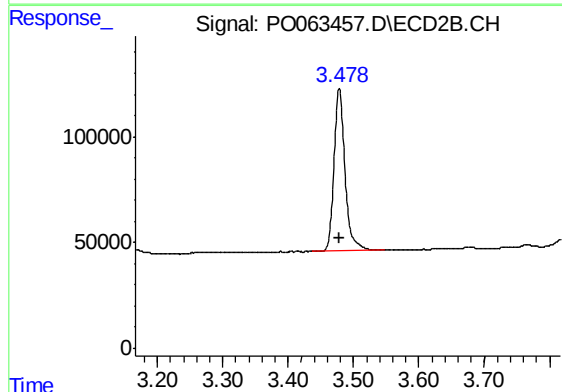


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: 0.000 min
Response: 892679
Conc: 16.35 ng/ml

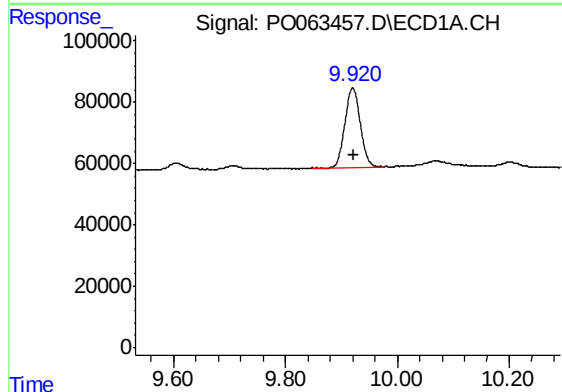

#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.002 min
Response: 494772
Conc: 8.50 ng/ml

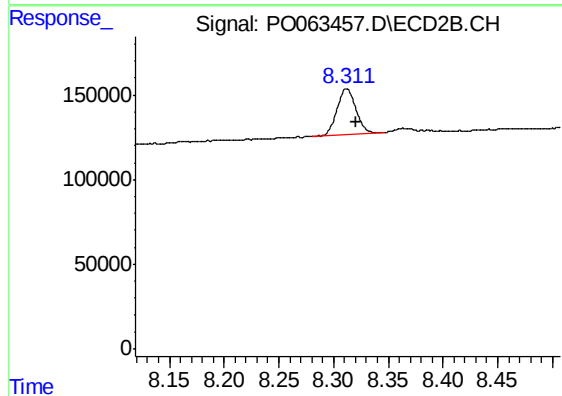

#2 Decachlorobiphenyl

R.T.: 8.312 min
Delta R.T.: -0.009 min
Response: 326943
Conc: 7.65 ng/ml