

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110219\
 Data File : P0063461.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2019 11:11
 Operator : HP/AJ
 Sample : K5640-02RE
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S6-02-ARE

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:53:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:29:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.311	3.477	889815	899584	15.268m	16.472
2)	SA Decachlor...	9.922	8.314	476828	365009	8.195	8.538

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
Data File : PO063461.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2019 11:11
Operator : HP/AJ
Sample : K5640-02RE
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S6-02-ARE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:53:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:29:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

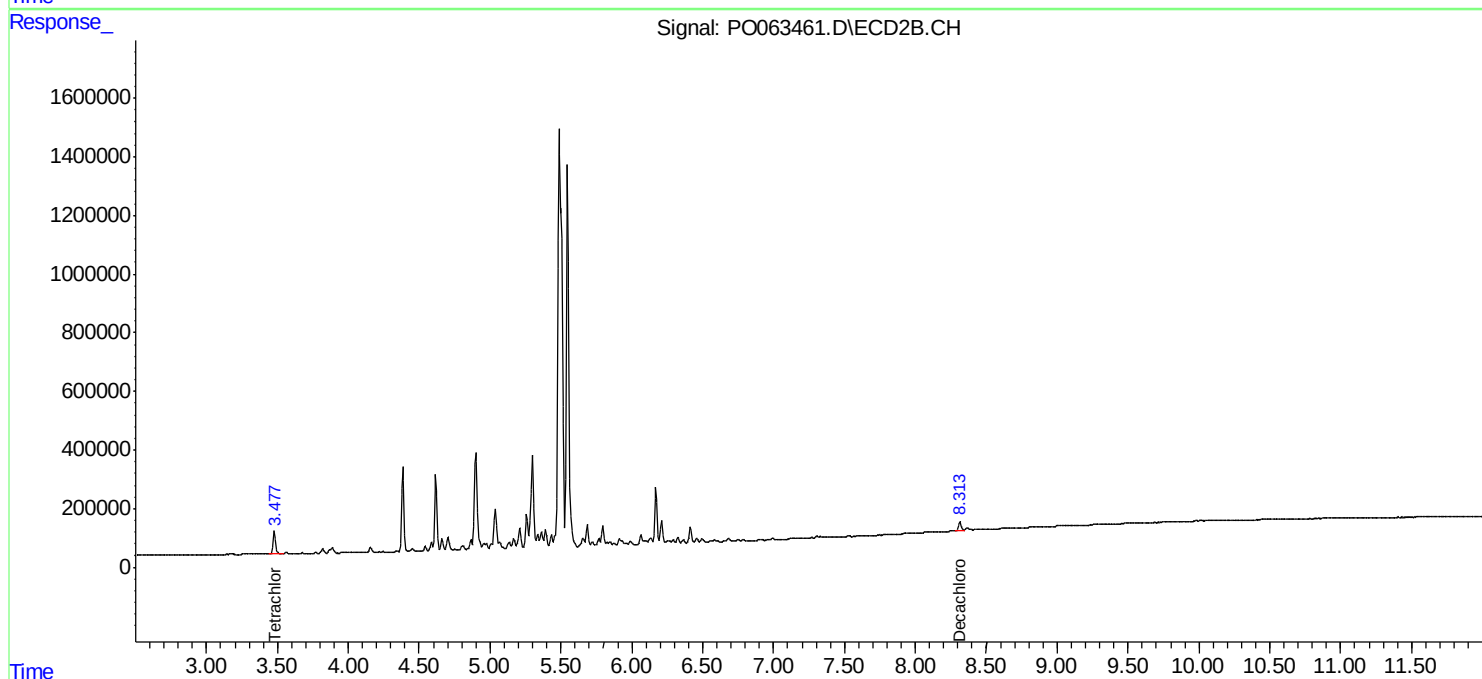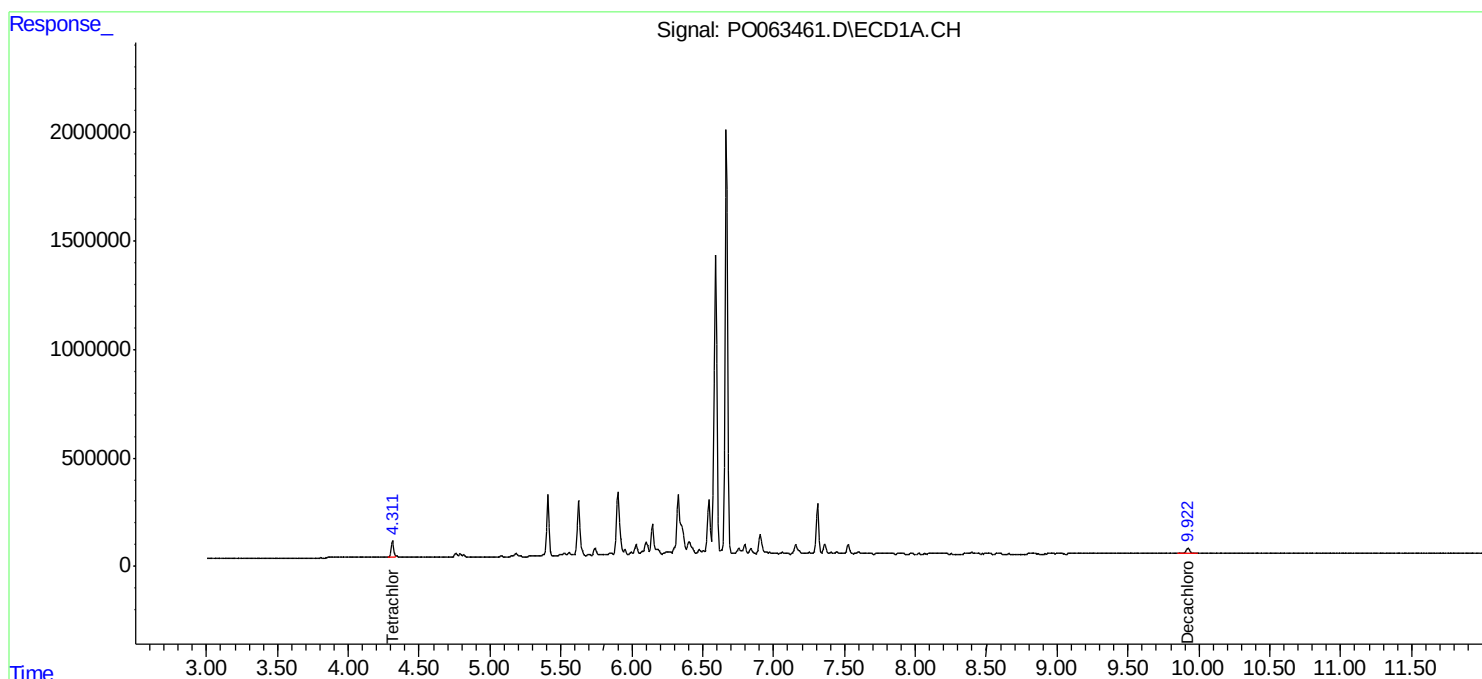

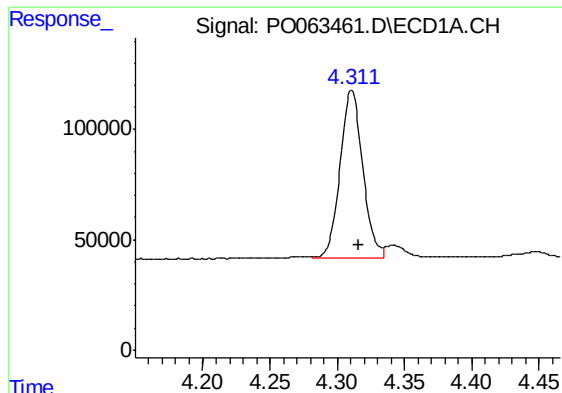


#1 Tetrachloro-m-xylene

R.T.: 4.311 min
Delta R.T.: -0.005 min
Response: 889815
Conc: 15.27 ng/ml m

Instrument :
ECD_O
ClientSampleId :
S6-02-ARE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:53:44 AM

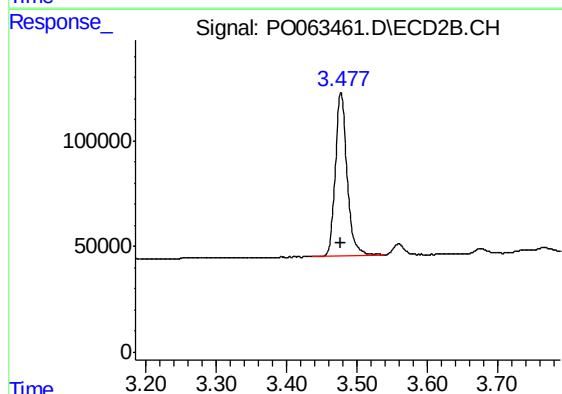


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 899584
Conc: 16.47 ng/ml

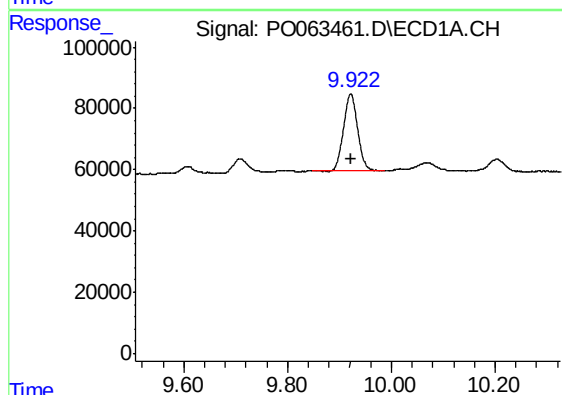

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: 0.000 min
Response: 476828
Conc: 8.20 ng/ml

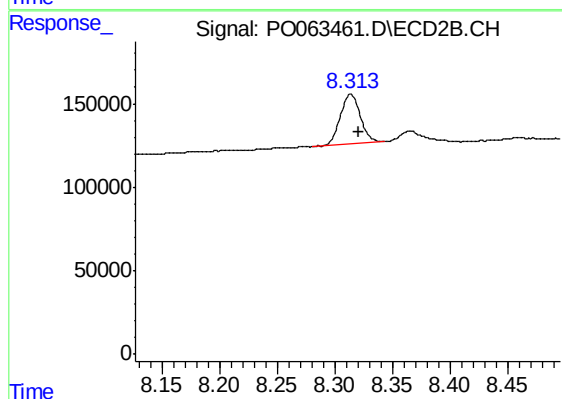

#2 Decachlorobiphenyl

R.T.: 8.314 min
Delta R.T.: -0.007 min
Response: 365009
Conc: 8.54 ng/ml