

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110219\
 Data File : P0063467.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 02 Nov 2019 13:23
 Operator : HP/AJ
 Sample : K5633-03DL 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S7-03-ADL

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:54:02 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:31:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.310	3.477	421540	424573	7.233	7.774
2)	SA Decachlor...	9.921	8.313	222600	134339	3.826m	3.142
Target Compounds							
31)	L7 AR-1260-1	7.058	5.952	2073580	2001133	668.649	724.563
32)	L7 AR-1260-2	7.312	6.139	3474814	3185937	860.752	830.347
33)	L7 AR-1260-3	7.670	6.286	2742018	2409352	853.818	767.888
34)	L7 AR-1260-4	7.895	6.747	2346239	2184435	734.954	862.765
35)	L7 AR-1260-5	8.206	6.989	5093343	5405978	868.458	886.893

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
Data File : PO063467.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 02 Nov 2019 13:23
Operator : HP/AJ
Sample : K5633-03DL 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S7-03-ADL


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:02 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:31:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

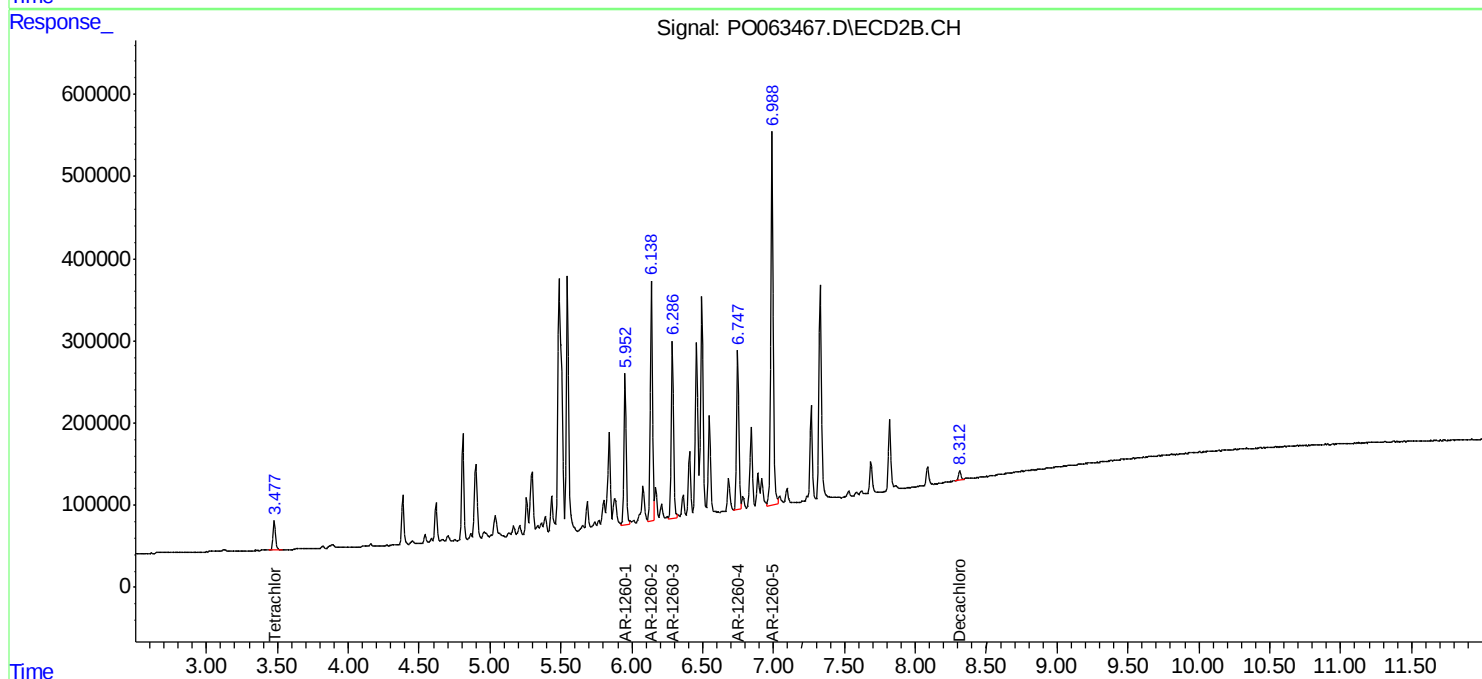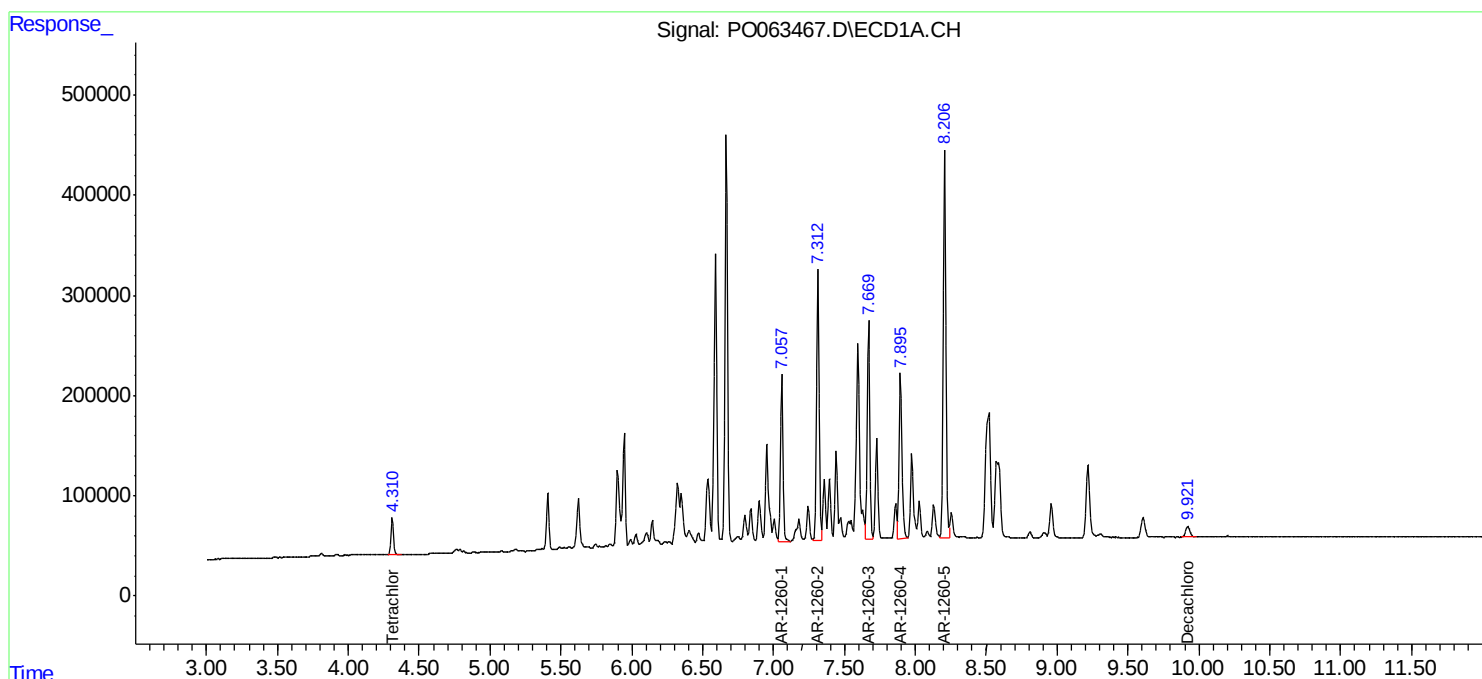

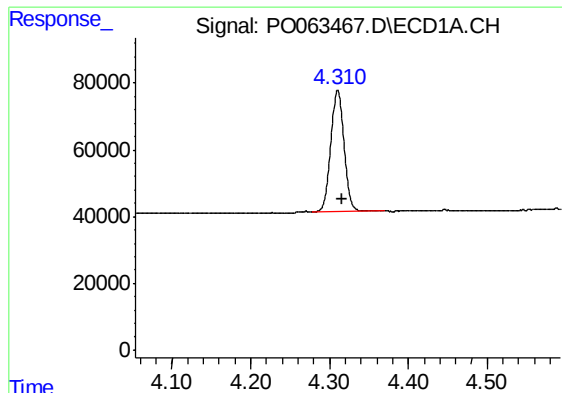


#1 Tetrachloro-m-xylene

R.T.: 4.310 min
Delta R.T.: -0.006 min
Response: 421540
Conc: 7.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-03-ADL


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:02 AM

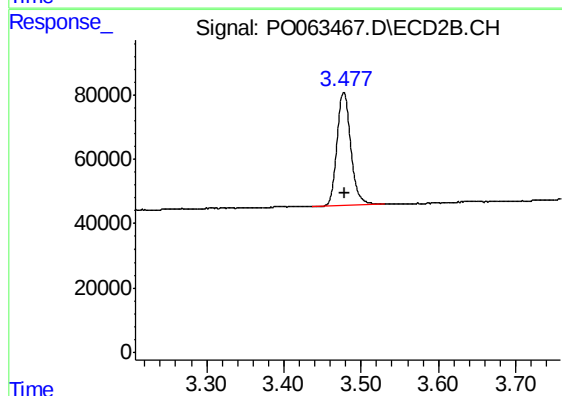


#1 Tetrachloro-m-xylene

R.T.: 3.477 min
Delta R.T.: 0.000 min
Response: 424573
Conc: 7.77 ng/ml

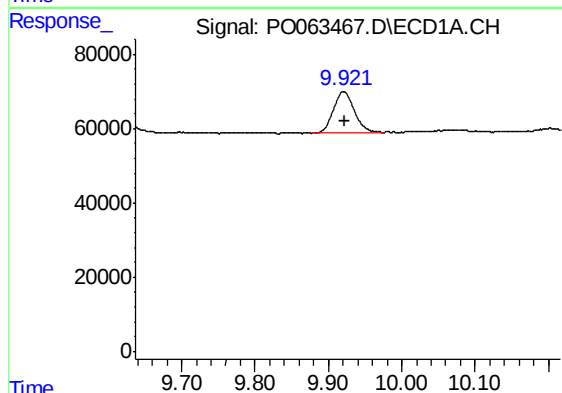


#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.002 min
Response: 222600
Conc: 3.83 ng/ml m

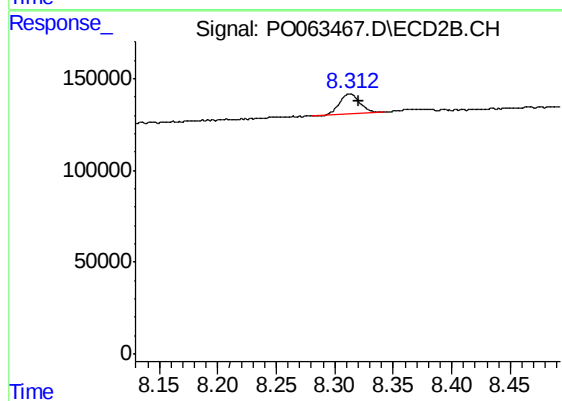

#2 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.008 min
Response: 134339
Conc: 3.14 ng/ml

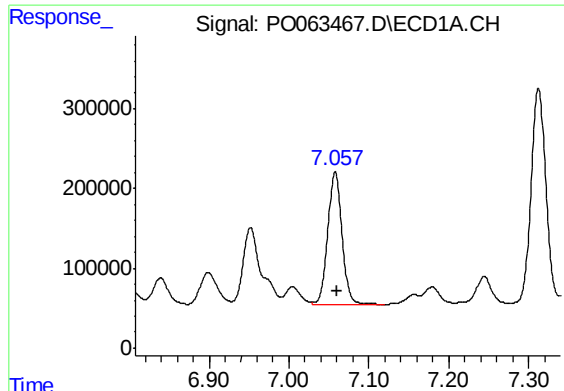


#31 AR-1260-1

R.T.: 7.058 min
Delta R.T.: -0.002 min
Response: 2073580
Conc: 668.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-03-ADL


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:02 AM

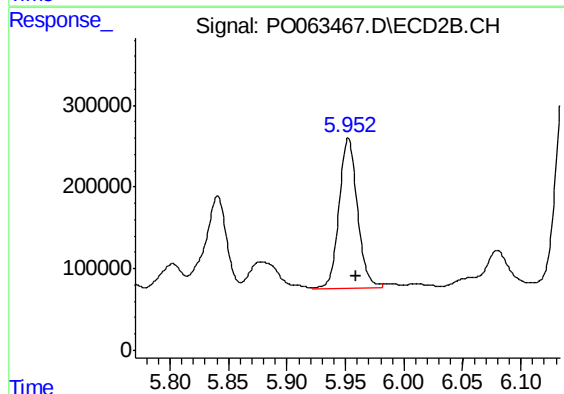


#31 AR-1260-1

R.T.: 5.952 min
Delta R.T.: -0.006 min
Response: 2001133
Conc: 724.56 ng/ml

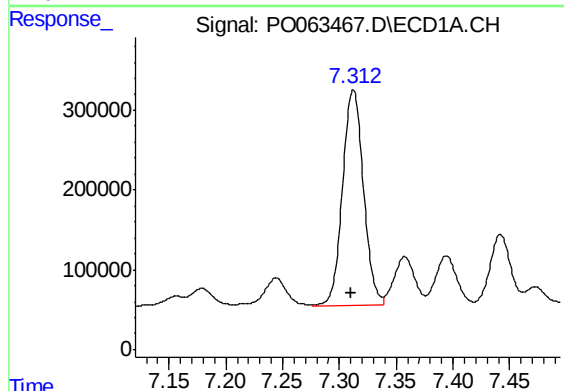


#32 AR-1260-2

R.T.: 7.312 min
Delta R.T.: 0.002 min
Response: 3474814
Conc: 860.75 ng/ml

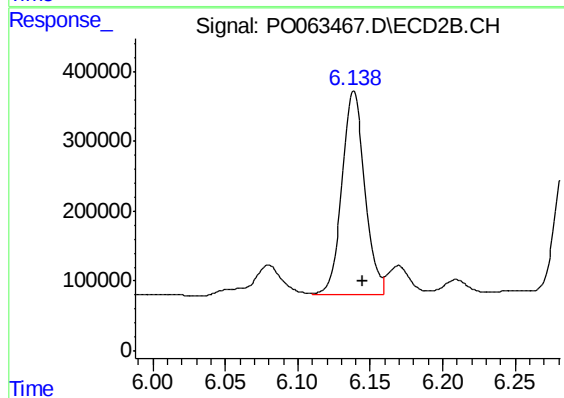

#32 AR-1260-2

R.T.: 6.139 min
Delta R.T.: -0.006 min
Response: 3185937
Conc: 830.35 ng/ml

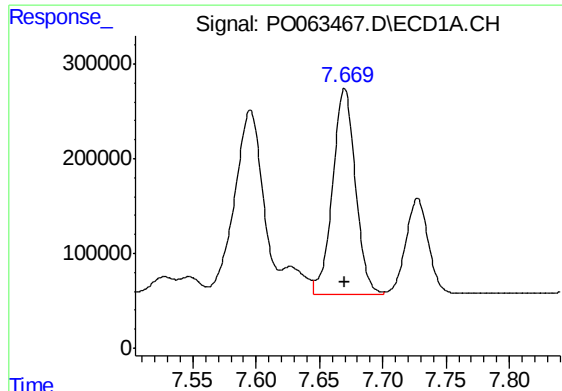


#33 AR-1260-3

R.T.: 7.670 min
Delta R.T.: 0.000 min
Response: 2742018
Conc: 853.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-03-ADL


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:02 AM

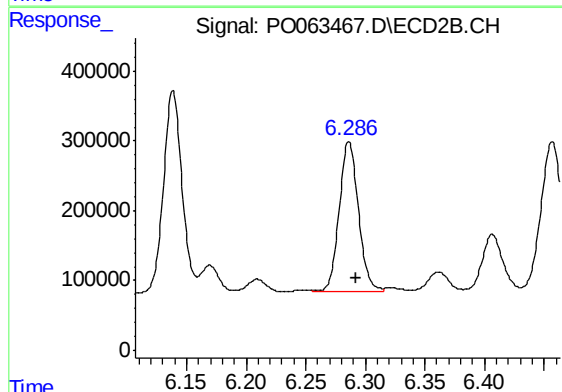


#33 AR-1260-3

R.T.: 6.286 min
Delta R.T.: -0.007 min
Response: 2409352
Conc: 767.89 ng/ml

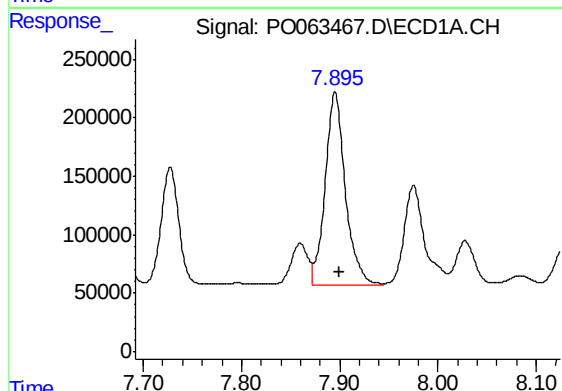


#34 AR-1260-4

R.T.: 7.895 min
Delta R.T.: -0.005 min
Response: 2346239
Conc: 734.95 ng/ml

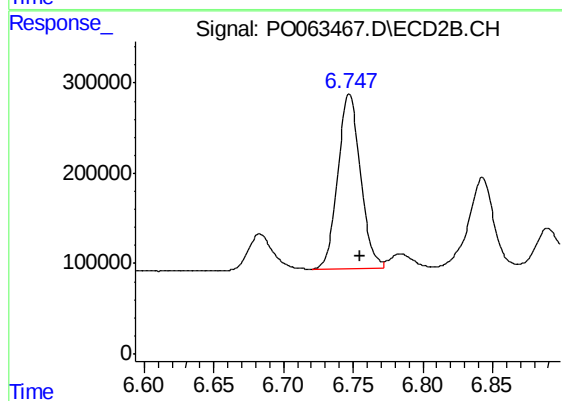

#34 AR-1260-4

R.T.: 6.747 min
Delta R.T.: -0.008 min
Response: 2184435
Conc: 862.76 ng/ml

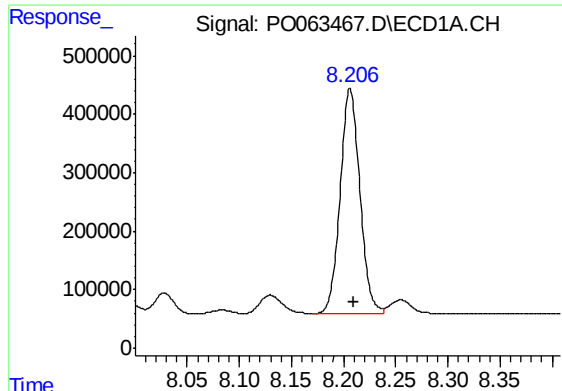


#35 AR-1260-5

R.T.: 8.206 min
Delta R.T.: -0.004 min
Response: 5093343
Conc: 868.46 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-03-ADL

Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:02 AM

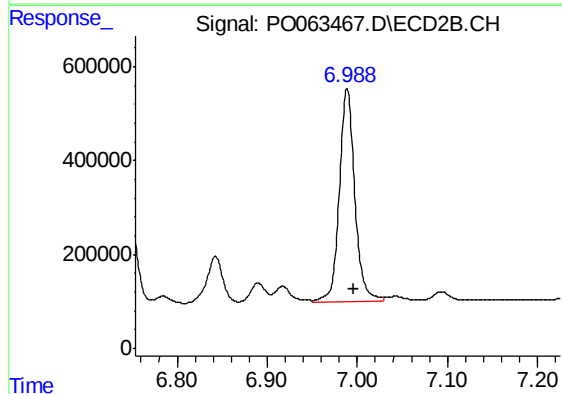

#35 AR-1260-5

R.T.: 6.989 min
Delta R.T.: -0.007 min
Response: 5405978
Conc: 886.89 ng/ml