

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110219\
Data File : P0063502.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2019 00:09
Operator : HP/AJ
Sample : K5642-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S1-10-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:44:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.311	3.478	1101223	1133651	18.895	20.758
2)	SA Decachlor...	9.921	8.313	566856	356963	9.742	8.350

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
Data File : PO063502.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2019 00:09
Operator : HP/AJ
Sample : K5642-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S1-10-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:44:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

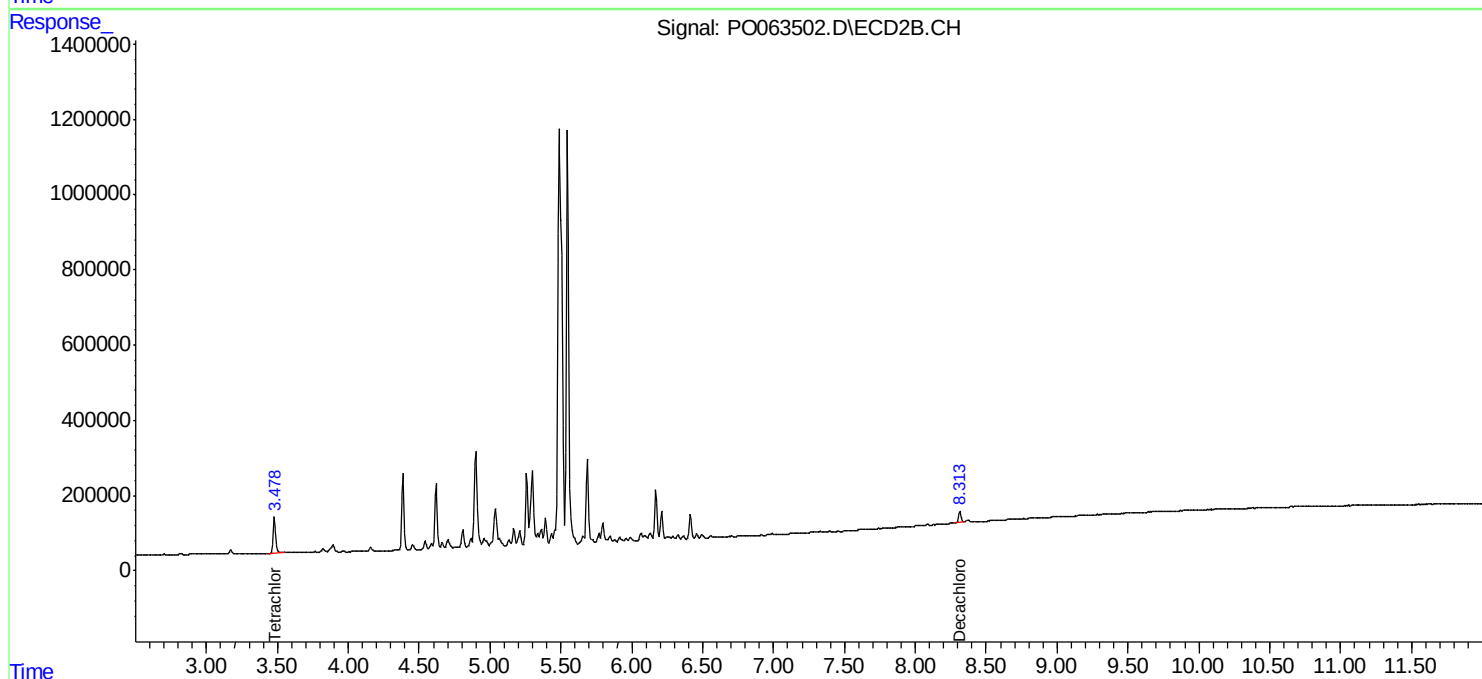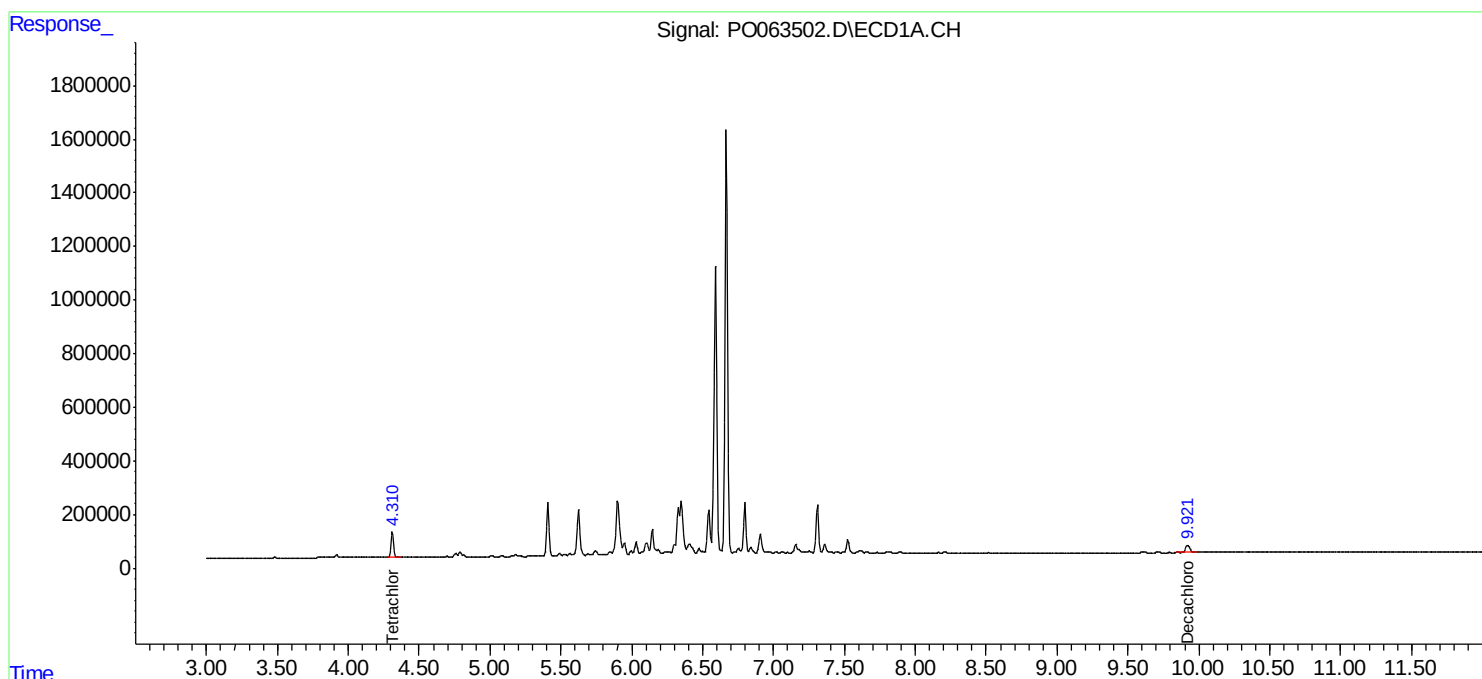


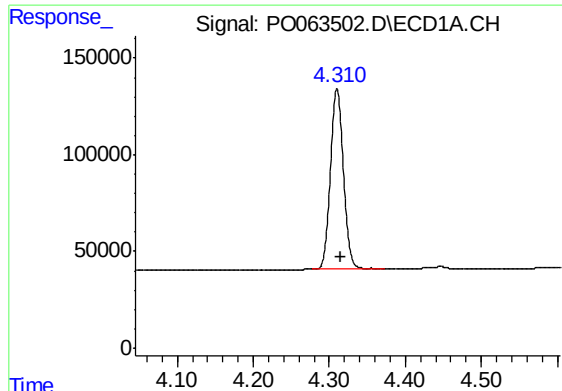

#1 Tetrachloro-m-xylene


R.T.: 4.311 min
Delta R.T.: -0.005 min
Response: 1101223
Conc: 18.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
S1-10-A

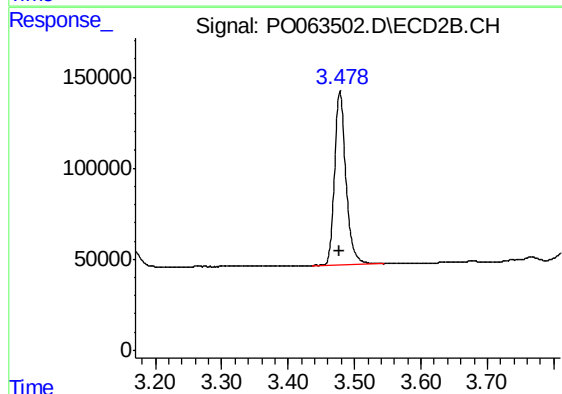


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: 0.000 min
Response: 1133651
Conc: 20.76 ng/ml

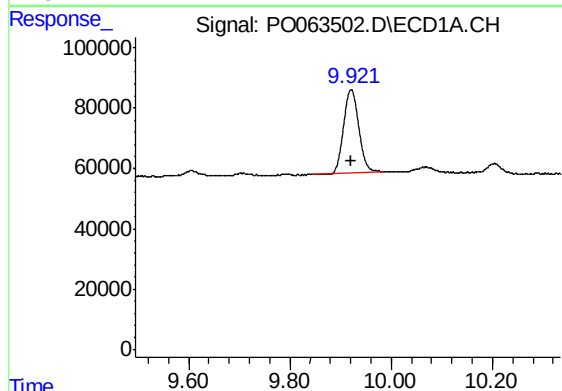

#2 Decachlorobiphenyl

R.T.: 9.921 min
Delta R.T.: -0.001 min
Response: 566856
Conc: 9.74 ng/ml

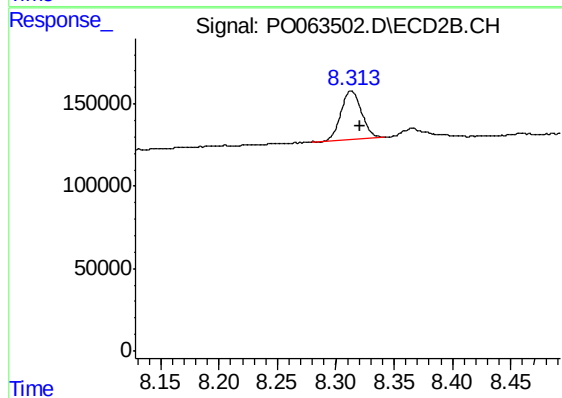

#2 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.008 min
Response: 356963
Conc: 8.35 ng/ml