

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
 Data File : P0063506.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2019 1:05
 Operator : HP/AJ
 Sample : K5607-01 10X
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OILY-WATER

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:54:37 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:46:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.308	3.478	85977	81176	1.475m	1.486
2)	SA Decachlor...	9.922	8.311	58272	40995	1.002m	0.959

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
Data File : PO063506.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2019 1:05
Operator : HP/AJ
Sample : K5607-01 10X
Misc :
ALS Vial : 53 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:46:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

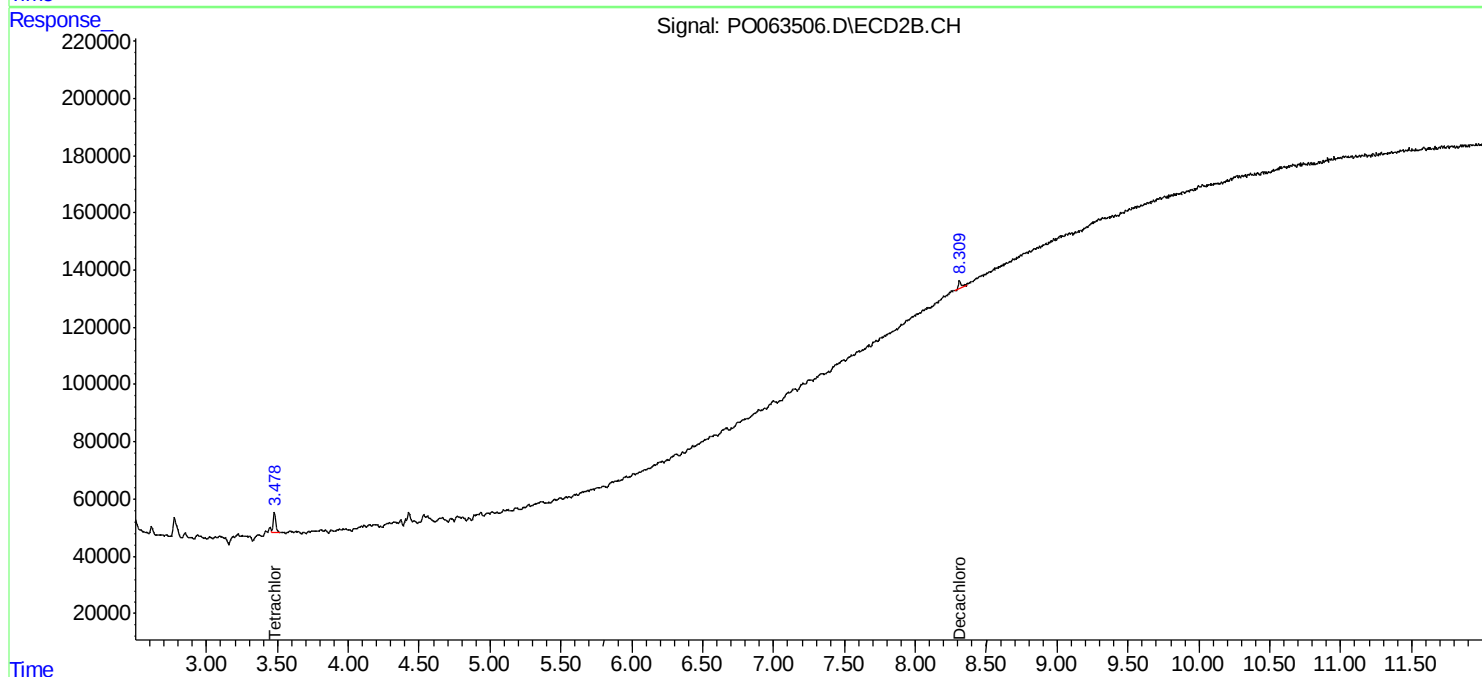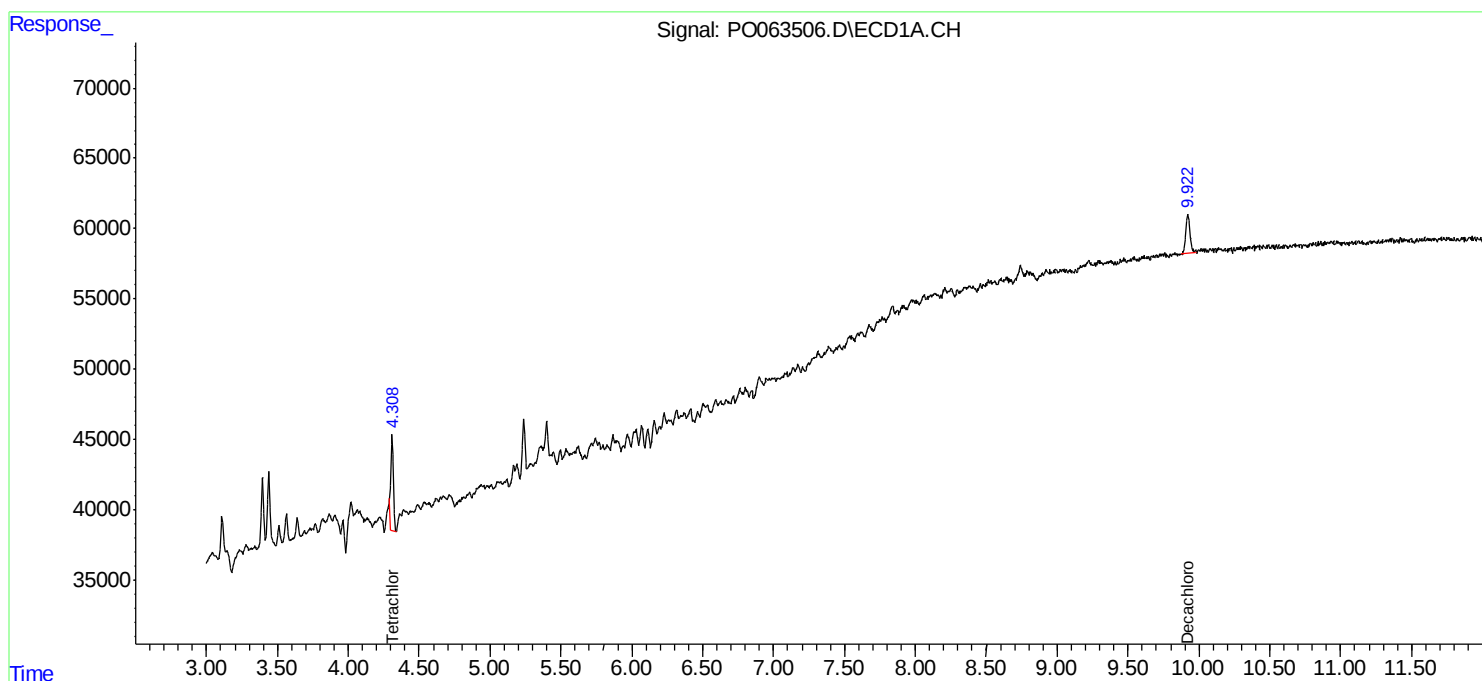

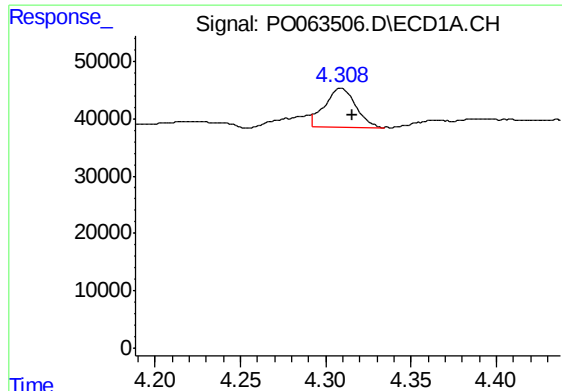


#1 Tetrachloro-m-xylene

R.T.: 4.308 min
Delta R.T.: -0.008 min
Response: 85977
Conc: 1.48 ng/ml m

Instrument :
ECD_O
ClientSampleId :
OILY-WATER


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:37 AM

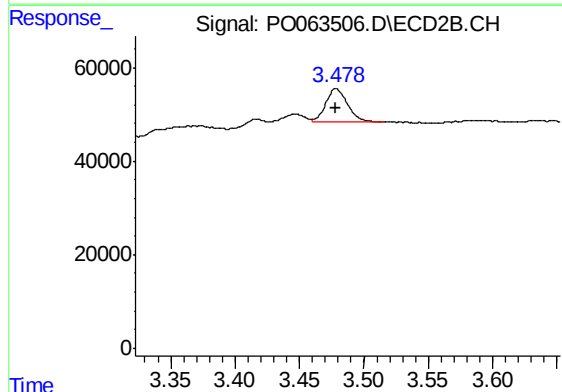


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: 0.000 min
Response: 81176
Conc: 1.49 ng/ml

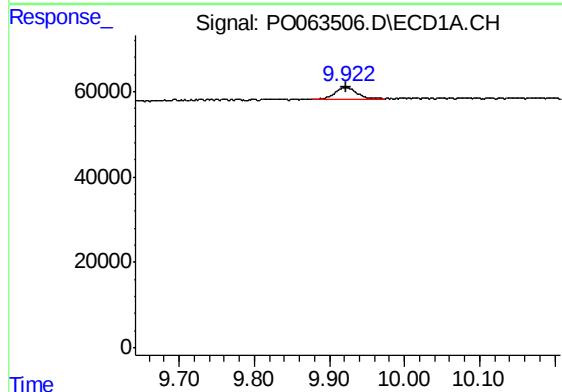

#2 Decachlorobiphenyl

R.T.: 9.922 min
Delta R.T.: 0.000 min
Response: 58272
Conc: 1.00 ng/ml m

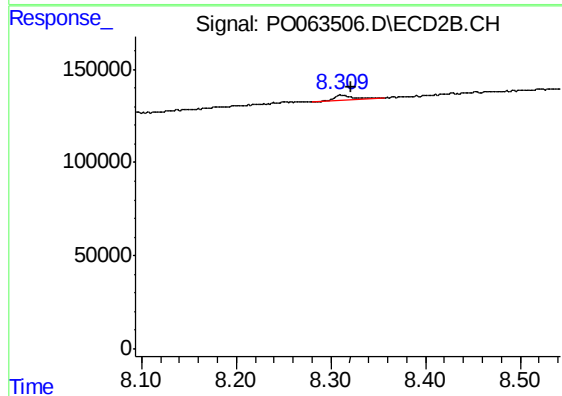

#2 Decachlorobiphenyl

R.T.: 8.311 min
Delta R.T.: -0.011 min
Response: 40995
Conc: 0.96 ng/ml