

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110219\
 Data File : P0063510.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2019 1:38
 Operator : HP/AJ
 Sample : K5623-02
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAT-TOTE

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:54:40 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:47:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.312	3.480	1081664	1055375	18.559m	19.324
2) SA Decachlor...	9.923	8.313	824090	582152	14.163	13.617

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
Data File : PO063510.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2019 1:38
Operator : HP/AJ
Sample : K5623-02
Misc :
ALS Vial : 55 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAT-TOTE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:40 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:47:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

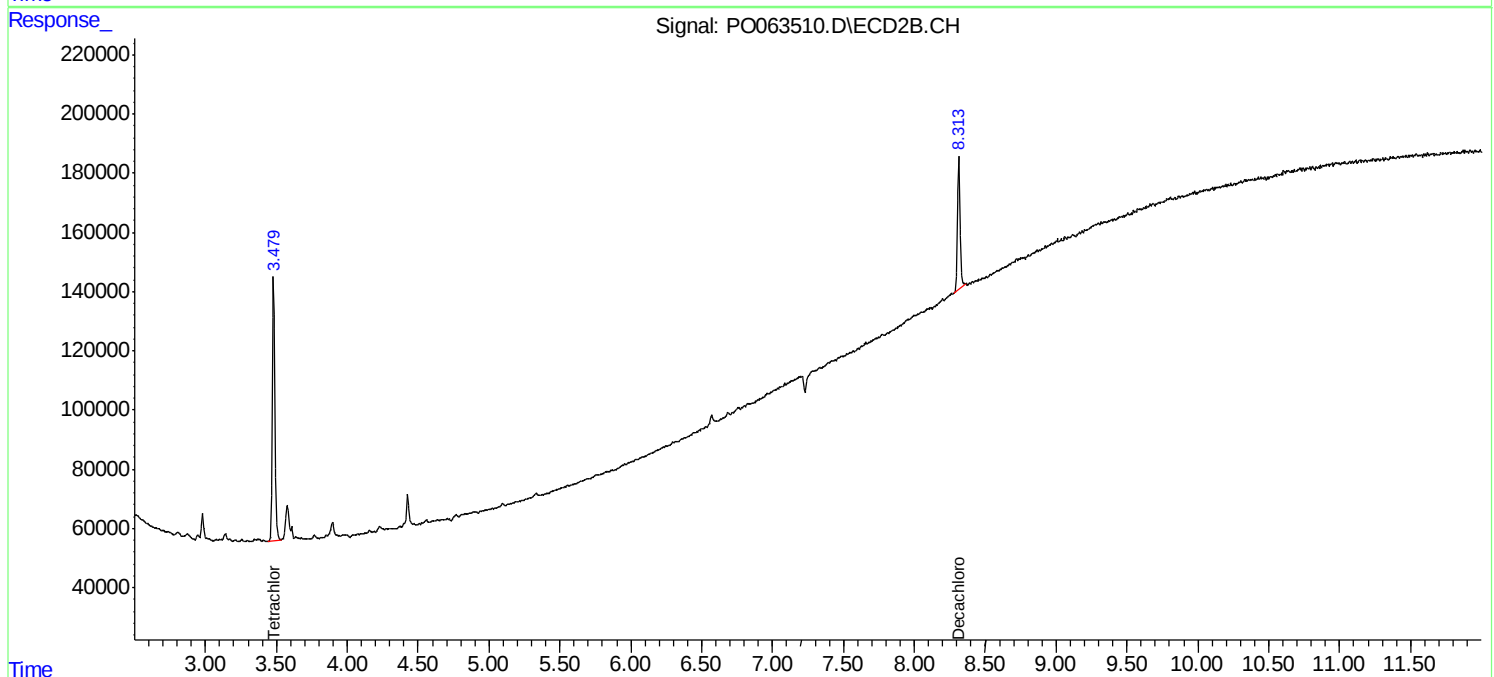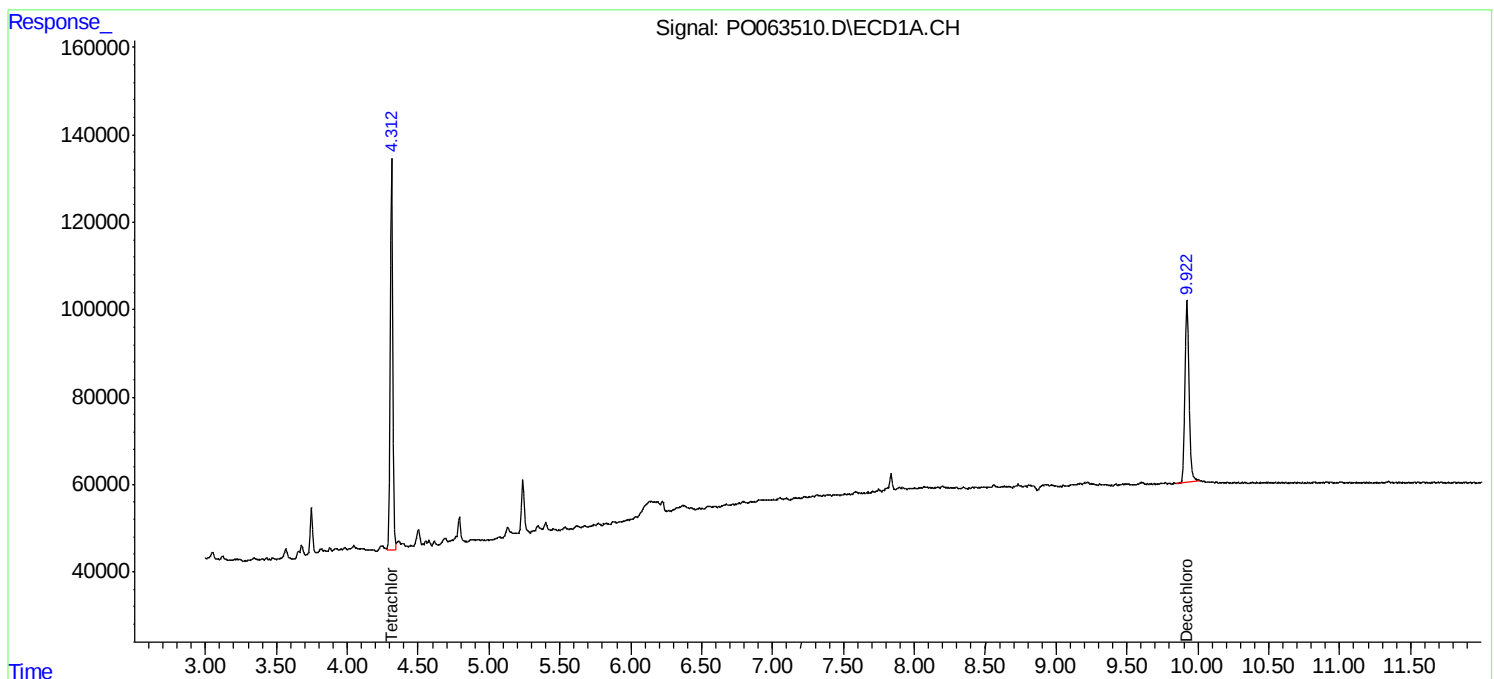

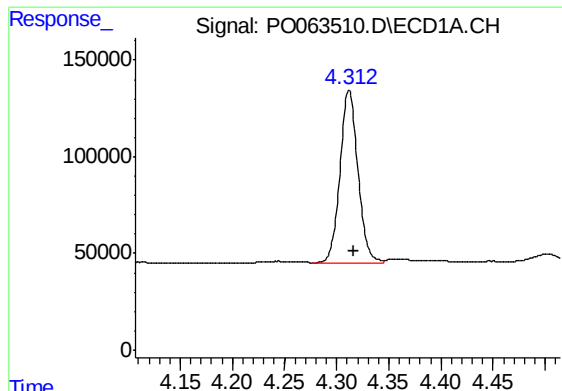


#1 Tetrachloro-m-xylene

R.T.: 4.312 min
Delta R.T.: -0.004 min
Response: 1081664
Conc: 18.56 ng/ml m

Instrument :
ECD_O
ClientSampleId :
PAT-TOTE


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:40 AM

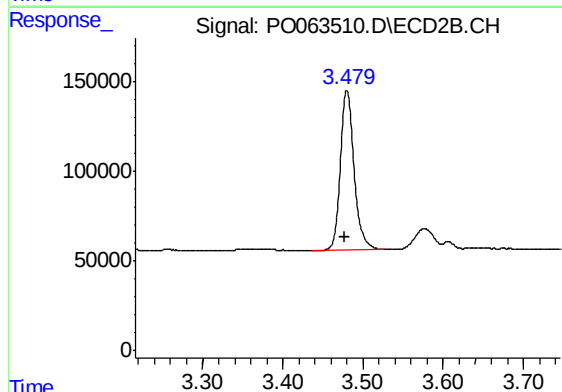


#1 Tetrachloro-m-xylene

R.T.: 3.480 min
Delta R.T.: 0.002 min
Response: 1055375
Conc: 19.32 ng/ml

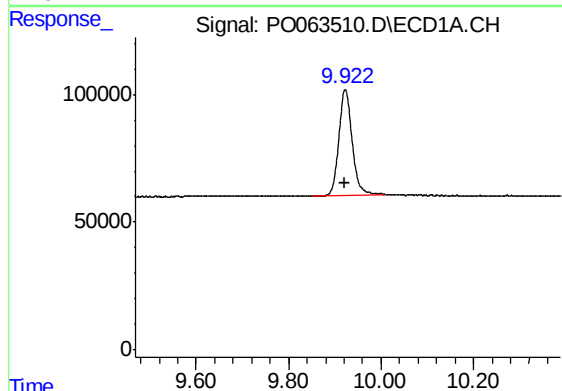

#2 Decachlorobiphenyl

R.T.: 9.923 min
Delta R.T.: 0.000 min
Response: 824090
Conc: 14.16 ng/ml

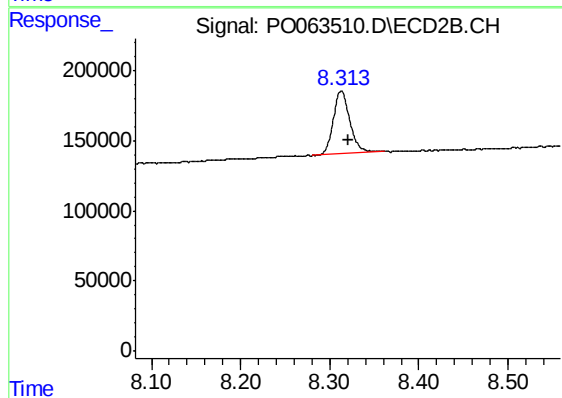

#2 Decachlorobiphenyl

R.T.: 8.313 min
Delta R.T.: -0.008 min
Response: 582152
Conc: 13.62 ng/ml