

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0110219\
 Data File : P0063512.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Nov 2019 1:55
 Operator : HP/AJ
 Sample : K5630-03
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S2-03-A

Manual Integrations
 APPROVED

Ankita
 11/4/2019 11:54:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 04 00:47:47 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0102919.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Oct 30 02:25:39 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.310	3.478	1157464	1214262	19.860	22.234
2) SA Decachlor...	9.920	8.314	764002	739021	13.131	17.286m#
Target Compounds						
31) L7 AR-1260-1	7.056	5.954	283264	410718	91.342	148.711 #
32) L7 AR-1260-2	7.309	6.139	1848974	590086	458.013	153.794 #
33) L7 AR-1260-3	7.669	6.286	403052	430495	125.504	137.204
34) L7 AR-1260-4	7.890	6.748	492919	269749	154.406	106.540 #
35) L7 AR-1260-5	8.206	6.989	583567	710093	99.503	116.496

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110219\
Data File : PO063512.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Nov 2019 1:55
Operator : HP/AJ
Sample : K5630-03
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
S2-03-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 04 00:47:47 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO102919.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Oct 30 02:25:39 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

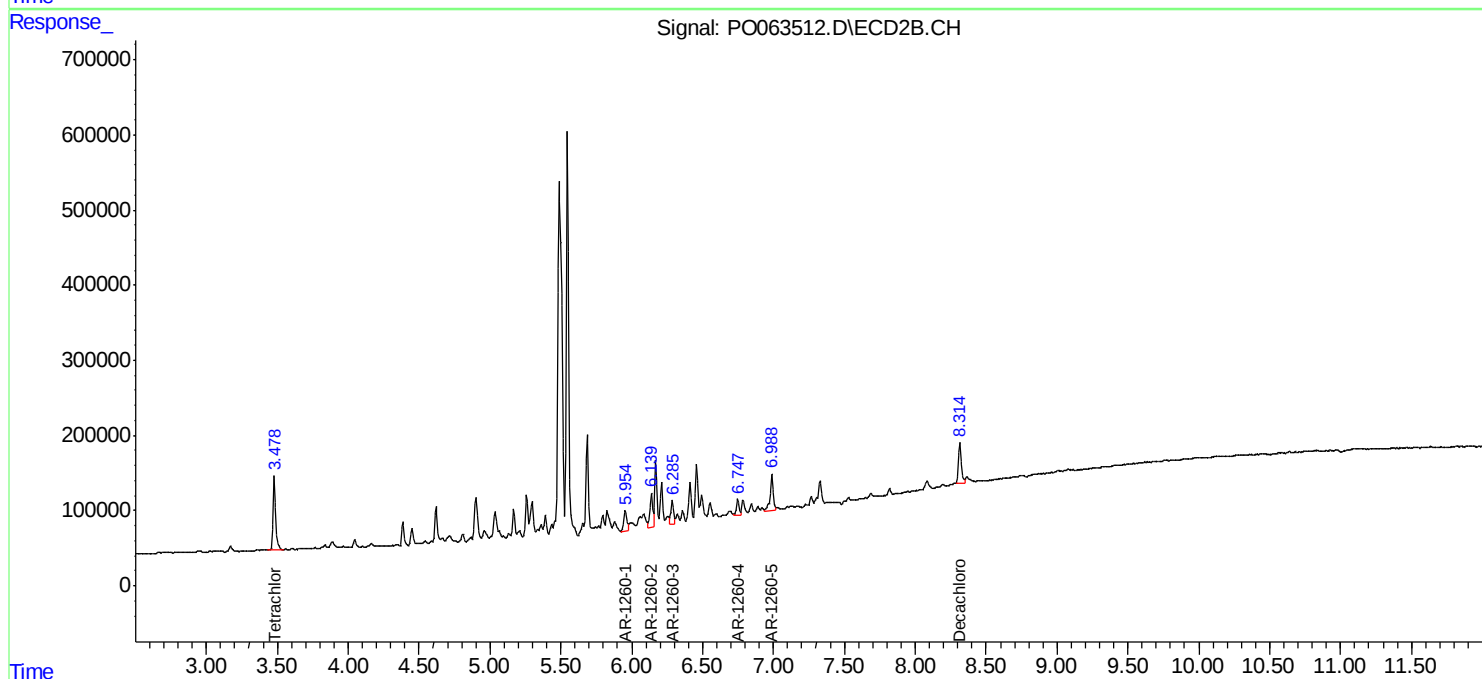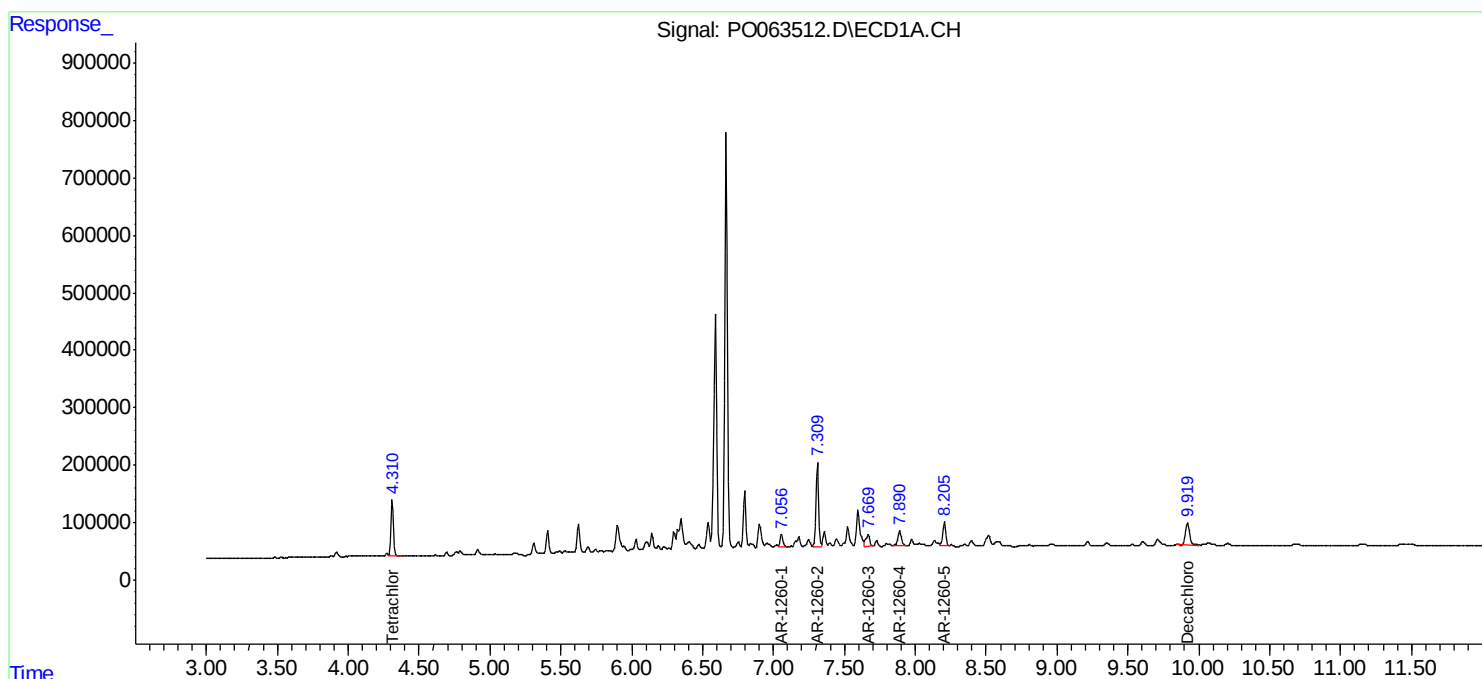

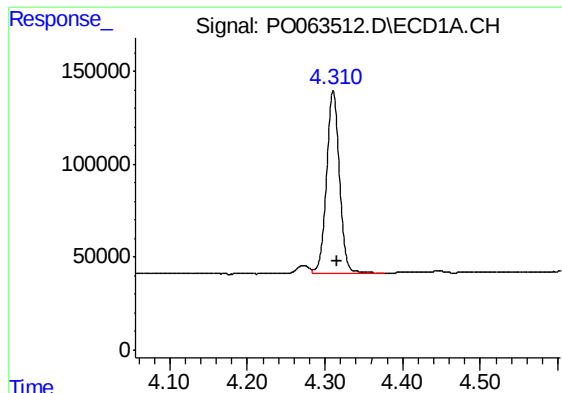


#1 Tetrachloro-m-xylene

R.T.: 4.310 min
Delta R.T.: -0.006 min
Response: 1157464
Conc: 19.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-03-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:44 AM

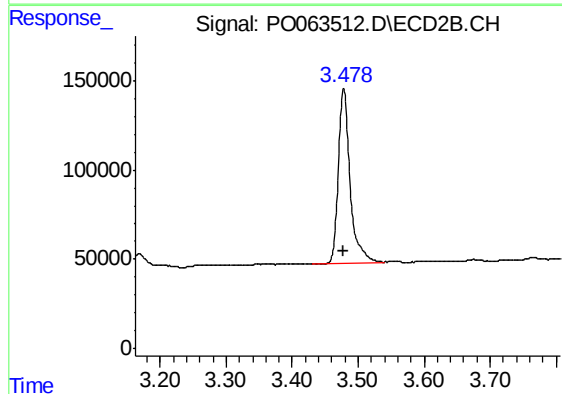


#1 Tetrachloro-m-xylene

R.T.: 3.478 min
Delta R.T.: 0.000 min
Response: 1214262
Conc: 22.23 ng/ml

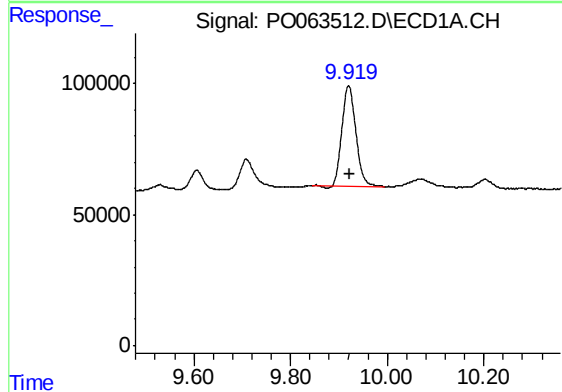


#2 Decachlorobiphenyl

R.T.: 9.920 min
Delta R.T.: -0.002 min
Response: 764002
Conc: 13.13 ng/ml

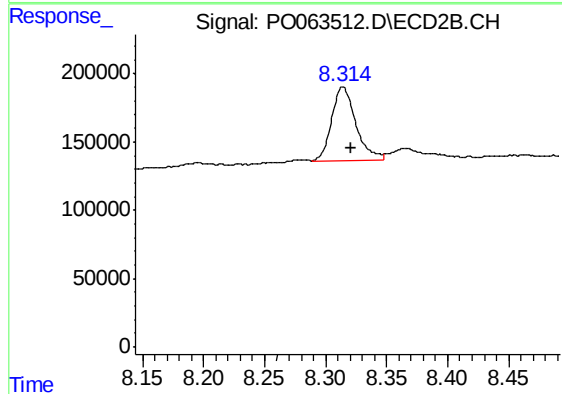

#2 Decachlorobiphenyl

R.T.: 8.314 min
Delta R.T.: -0.007 min
Response: 739021
Conc: 17.29 ng/ml m

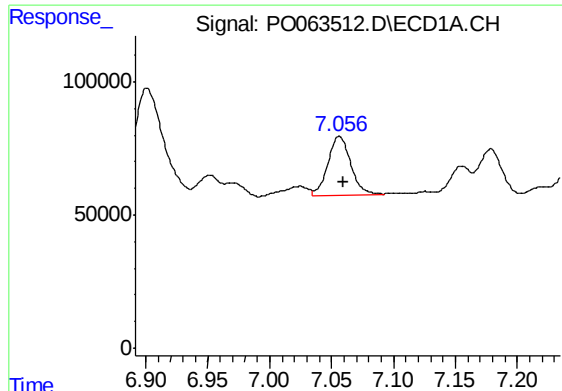


#31 AR-1260-1

R.T.: 7.056 min
Delta R.T.: -0.004 min
Response: 283264
Conc: 91.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-03-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:44 AM

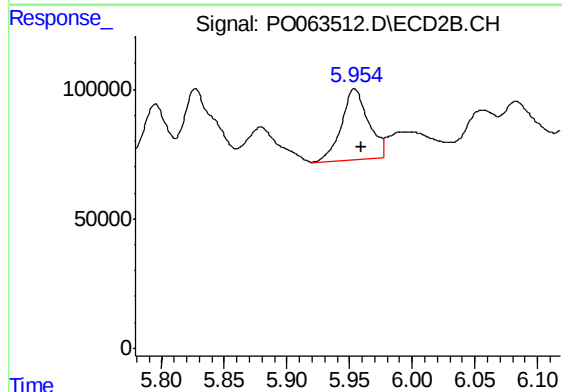


#31 AR-1260-1

R.T.: 5.954 min
Delta R.T.: -0.005 min
Response: 410718
Conc: 148.71 ng/ml

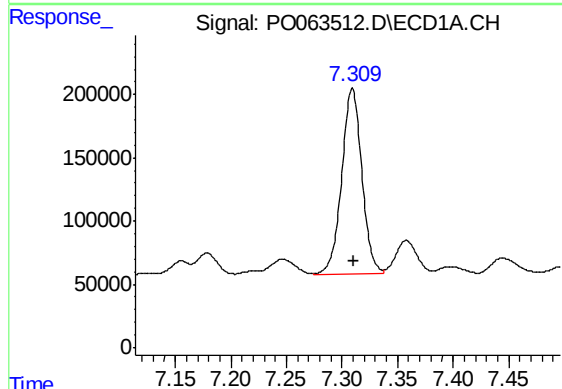


#32 AR-1260-2

R.T.: 7.309 min
Delta R.T.: 0.000 min
Response: 1848974
Conc: 458.01 ng/ml

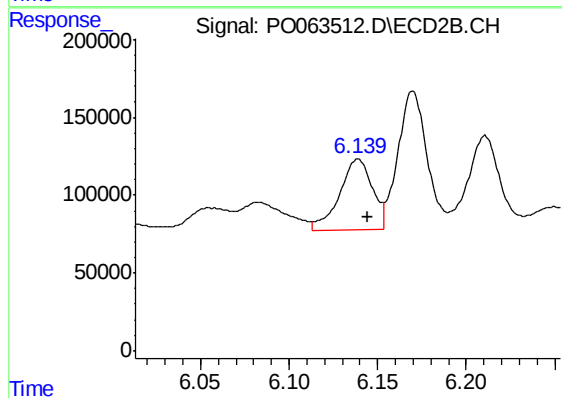

#32 AR-1260-2

R.T.: 6.139 min
Delta R.T.: -0.006 min
Response: 590086
Conc: 153.79 ng/ml

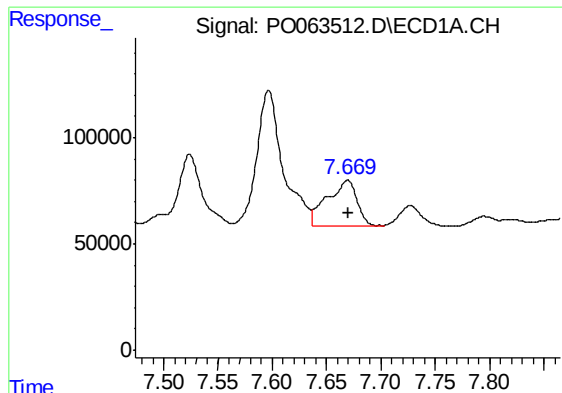


#33 AR-1260-3

R.T.: 7.669 min
Delta R.T.: -0.001 min
Response: 403052
Conc: 125.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-03-A


Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:44 AM

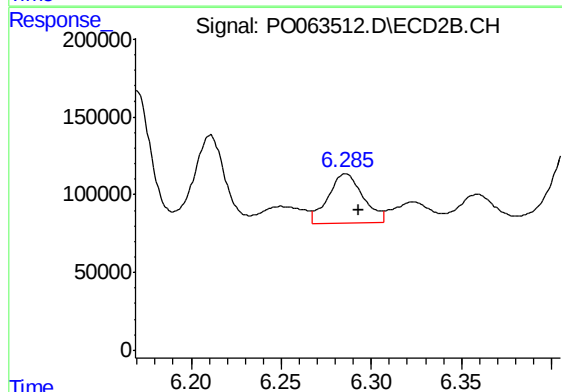


#33 AR-1260-3

R.T.: 6.286 min
Delta R.T.: -0.007 min
Response: 430495
Conc: 137.20 ng/ml

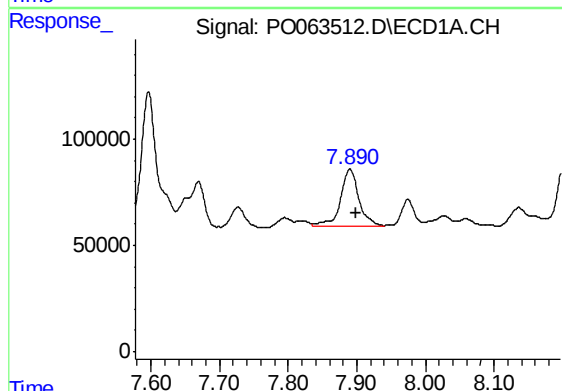


#34 AR-1260-4

R.T.: 7.890 min
Delta R.T.: -0.010 min
Response: 492919
Conc: 154.41 ng/ml

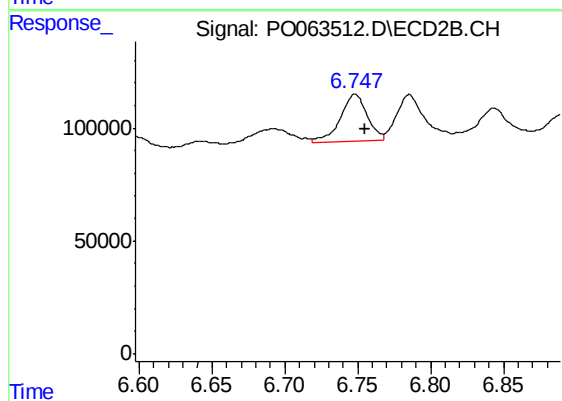

#34 AR-1260-4

R.T.: 6.748 min
Delta R.T.: -0.007 min
Response: 269749
Conc: 106.54 ng/ml

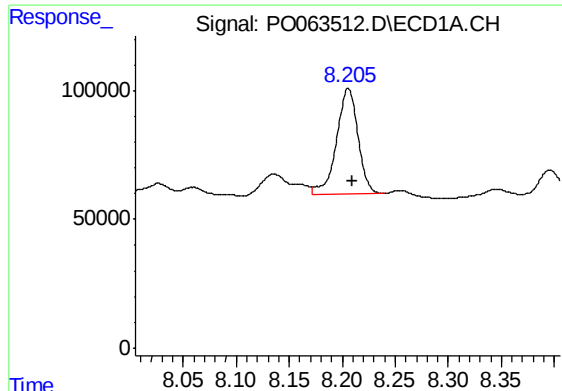


#35 AR-1260-5

R.T.: 8.206 min
Delta R.T.: -0.004 min
Response: 583567
Conc: 99.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
S2-03-A

Manual Integrations
APPROVED

Ankita
11/4/2019 11:54:44 AM

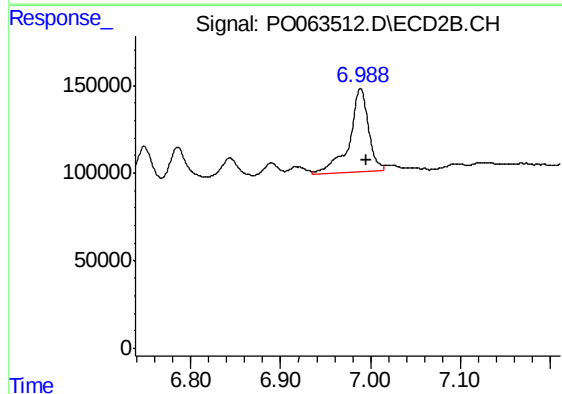

#35 AR-1260-5

R.T.: 6.989 min
Delta R.T.: -0.006 min
Response: 710093
Conc: 116.50 ng/ml