

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110618\
 Data File : P0051098.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 18:04
 Operator : SM/SJ
 Sample : J5810-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 110218-SIDI-E-D-M

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 02:43:18 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 06 00:37:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.353	3.342	7314288	3455523	19.605m	16.749m
2) SA Decachlor...	10.003	8.082	5542233	4108841	18.766	19.355

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110618\
Data File : PO051098.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 18:04
Operator : SM/SJ
Sample : J5810-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
110218-SIDI-E-D-M

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 02:43:18 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 00:37:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

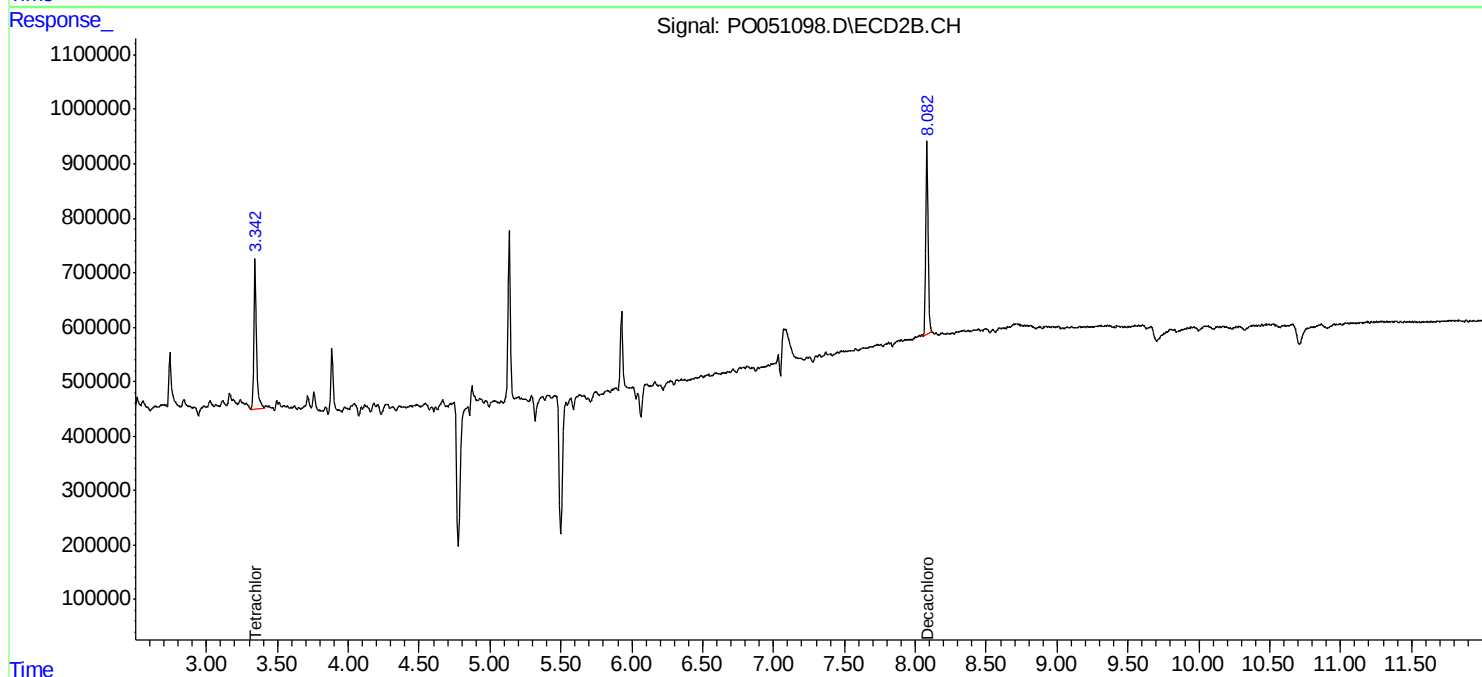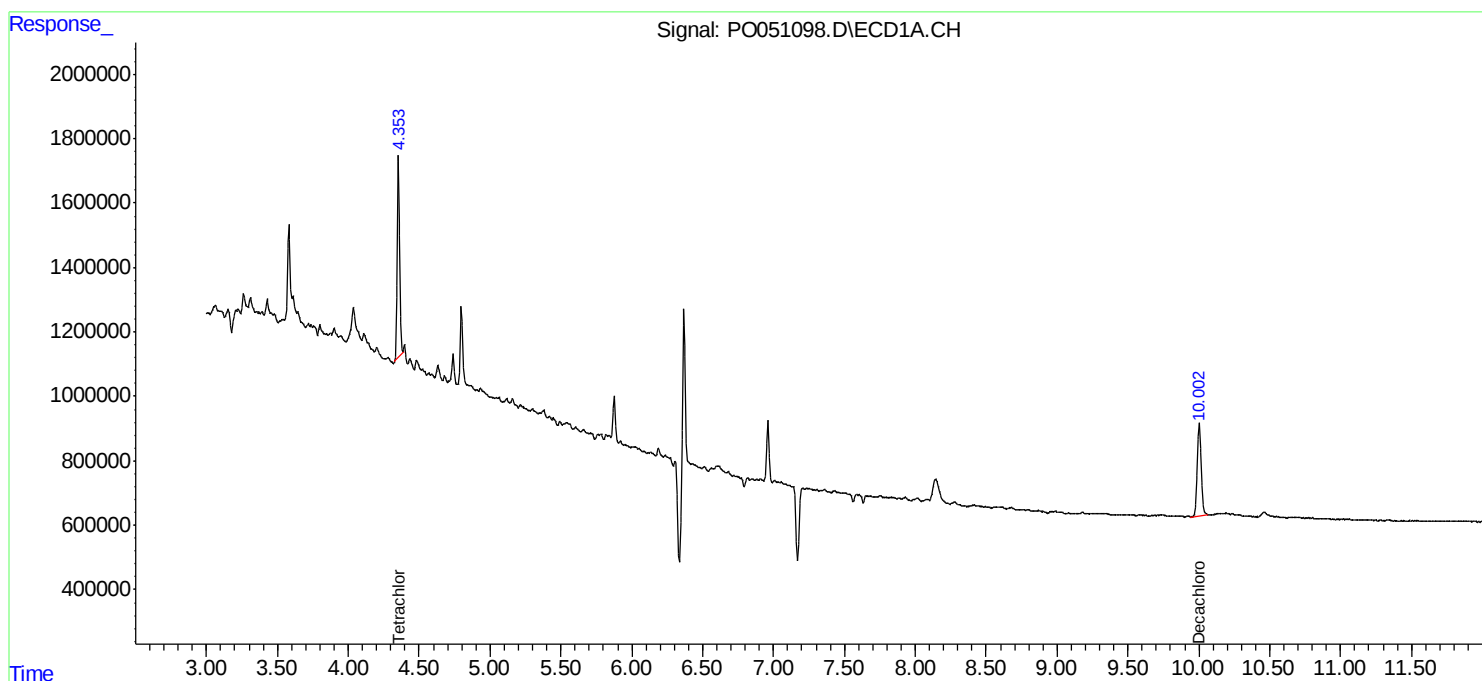


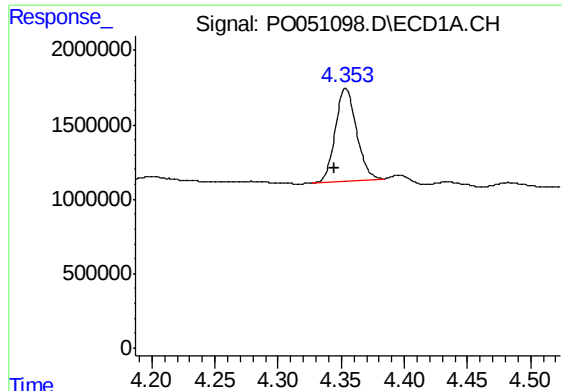

#1 Tetrachloro-m-xylene


R.T.: 4.353 min
Delta R.T.: 0.008 min
Response: 7314288
Conc: 19.61 ng/ml m

Instrument :
ECD_O
ClientSampleId :
110218-SIDI-E-D-M

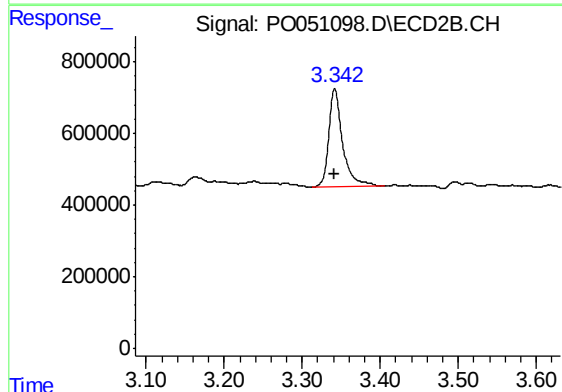


#1 Tetrachloro-m-xylene

R.T.: 3.342 min
Delta R.T.: 0.000 min
Response: 3455523
Conc: 16.75 ng/ml m

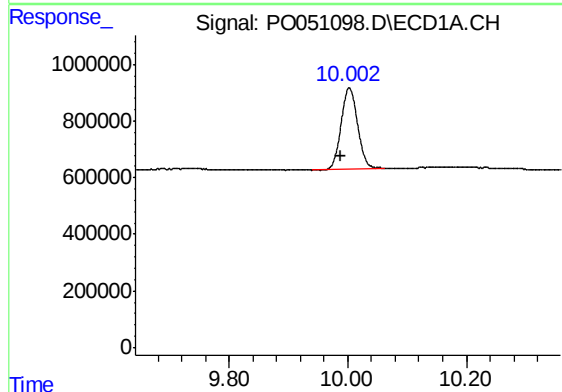

#2 Decachlorobiphenyl

R.T.: 10.003 min
Delta R.T.: 0.014 min
Response: 5542233
Conc: 18.77 ng/ml

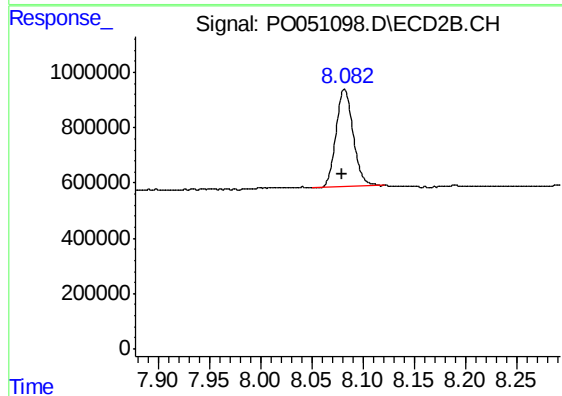

#2 Decachlorobiphenyl

R.T.: 8.082 min
Delta R.T.: 0.003 min
Response: 4108841
Conc: 19.35 ng/ml