

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110618\
 Data File : P0051104.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Nov 2018 19:46
 Operator : SM/SJ
 Sample : J5810-11
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 110218-TIPC-E-D-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 02:45:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 06 00:37:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.345	3.341	8927384	4149447	23.929m	20.113m
2)	SA Decachlor...	9.992	8.081	7394177	5443495	25.037	25.642

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110618\
Data File : PO051104.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Nov 2018 19:46
Operator : SM/SJ
Sample : J5810-11
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
110218-TIPC-E-D-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 02:45:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 00:37:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

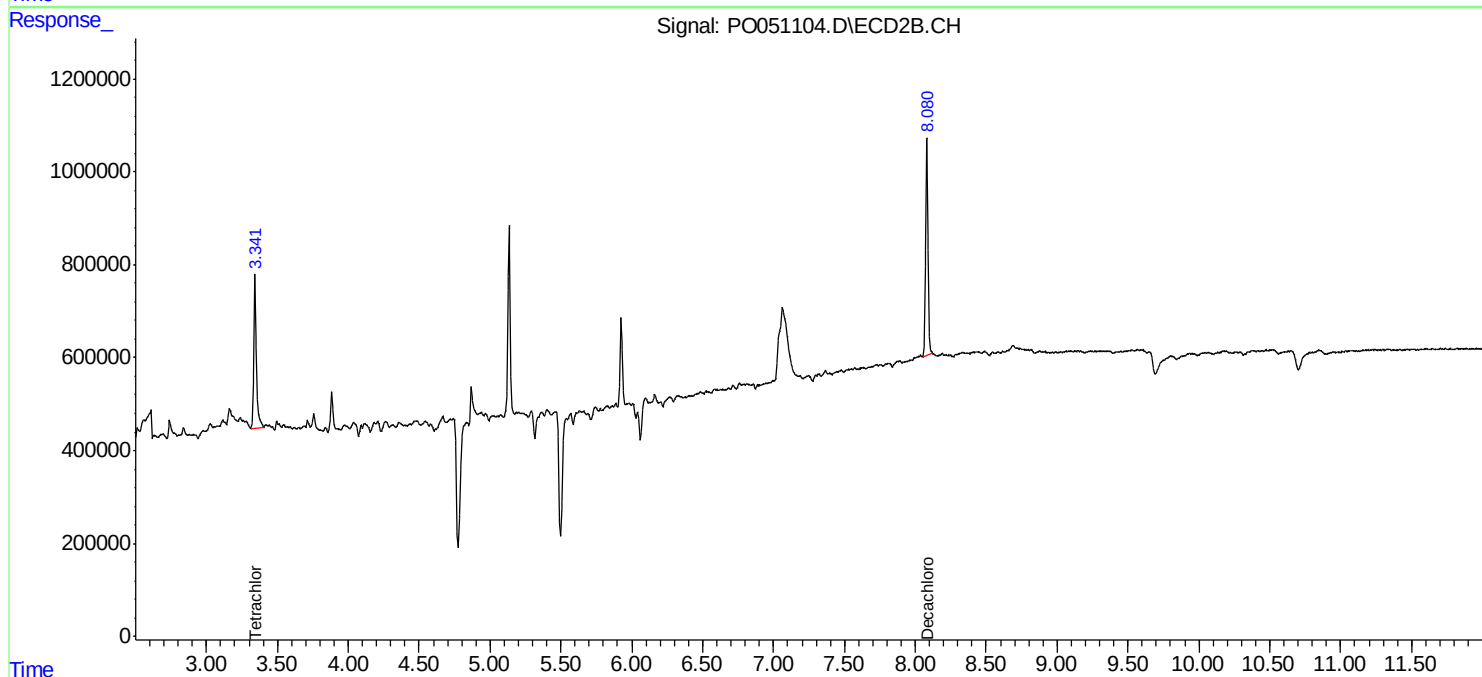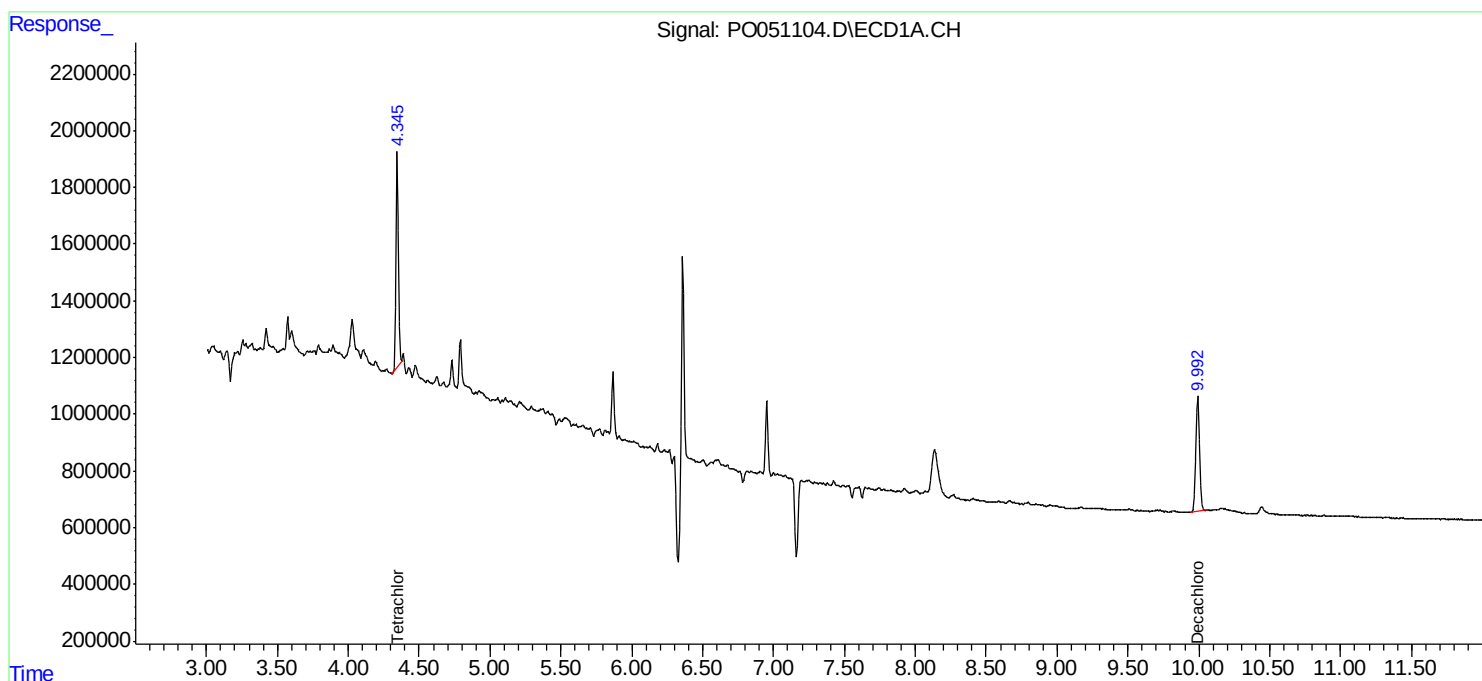


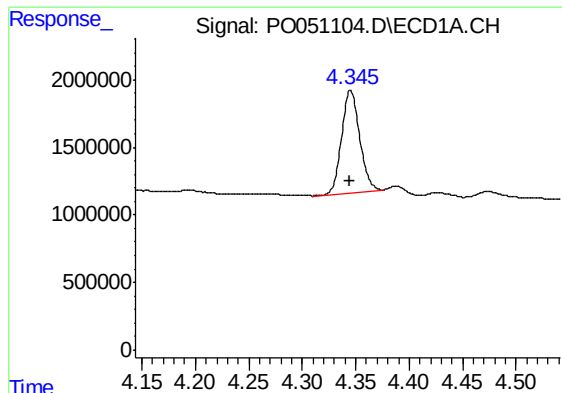

#1 Tetrachloro-m-xylene


R.T.: 4.345 min
Delta R.T.: 0.000 min
Response: 8927384
Conc: 23.93 ng/ml m

Instrument :
ECD_O
ClientSampleId :
110218-TIPC-E-D-S

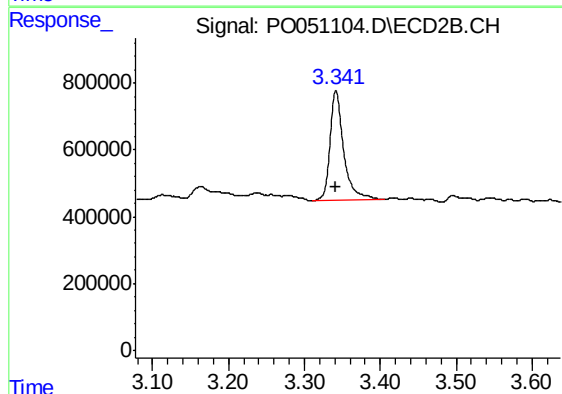


#1 Tetrachloro-m-xylene

R.T.: 3.341 min
Delta R.T.: 0.000 min
Response: 4149447
Conc: 20.11 ng/ml m

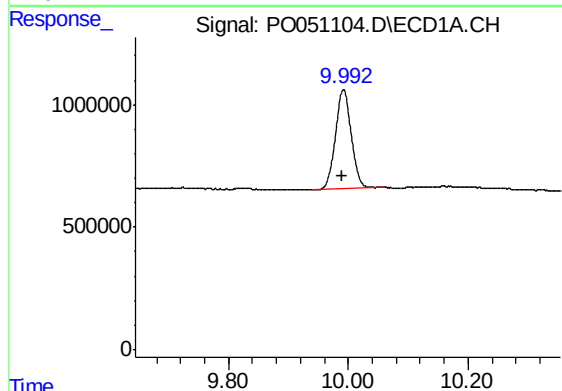

#2 Decachlorobiphenyl

R.T.: 9.992 min
Delta R.T.: 0.003 min
Response: 7394177
Conc: 25.04 ng/ml

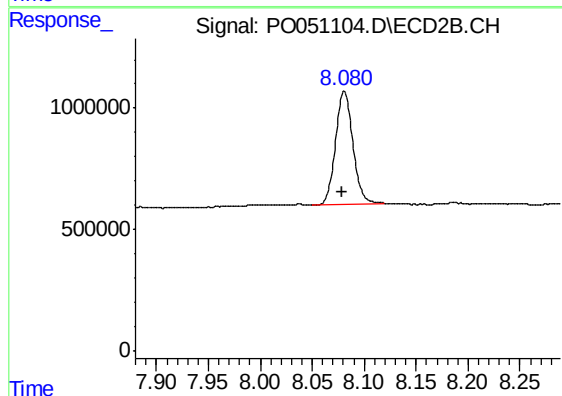

#2 Decachlorobiphenyl

R.T.: 8.081 min
Delta R.T.: 0.002 min
Response: 5443495
Conc: 25.64 ng/ml