

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110718\
 Data File : PO051153.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Nov 2018 12:42
 Operator : SM/SJ
 Sample : J5824-01 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 A366481

Manual Integrations
 APPROVED

Sohil
 11/7/2018 4:26:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 14:54:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 06 00:37:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.344	3.343	1582547	403539	4.242	1.990m#
2) SA Decachlor...	9.997	8.080	722063	676756	2.428m	3.056 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110718\
Data File : PO051153.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Nov 2018 12:42
Operator : SM/SJ
Sample : J5824-01 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
A366481


Manual Integrations
APPROVED

Sohil
11/7/2018 4:26:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 14:54:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 00:37:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

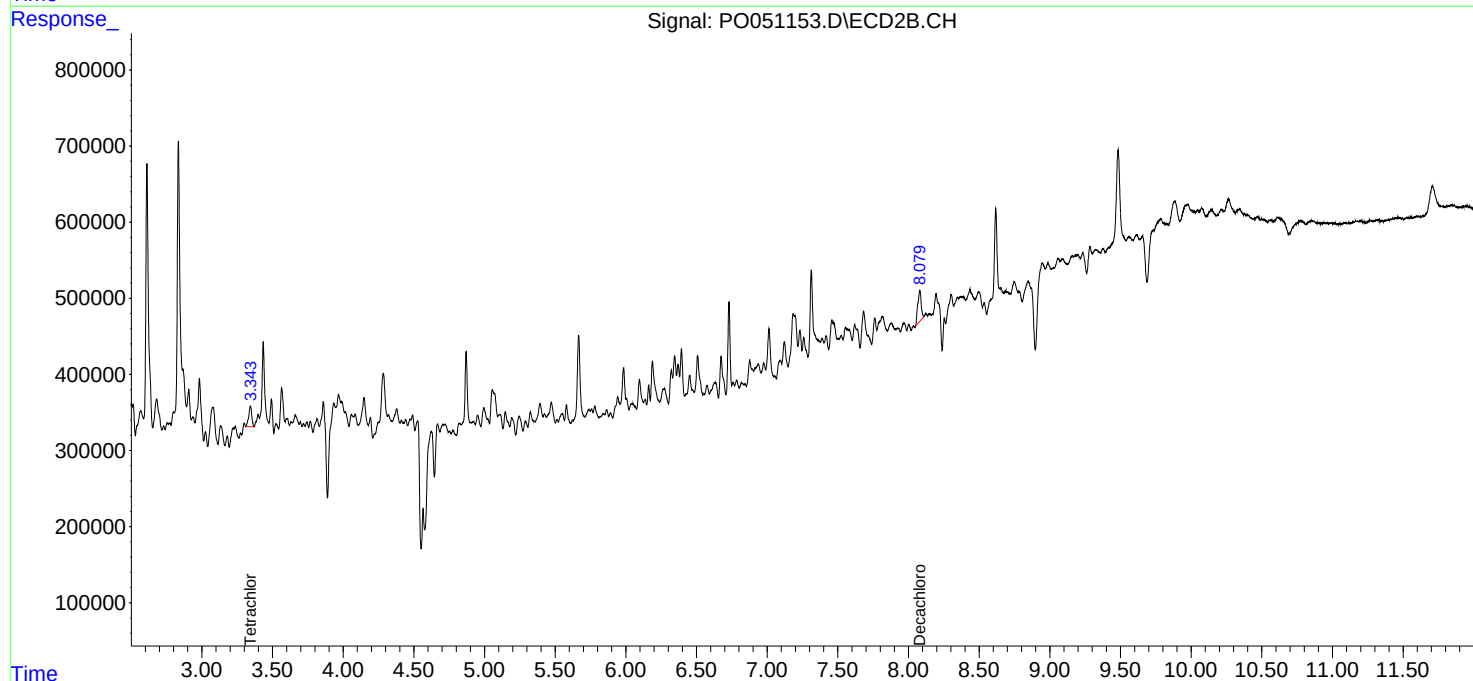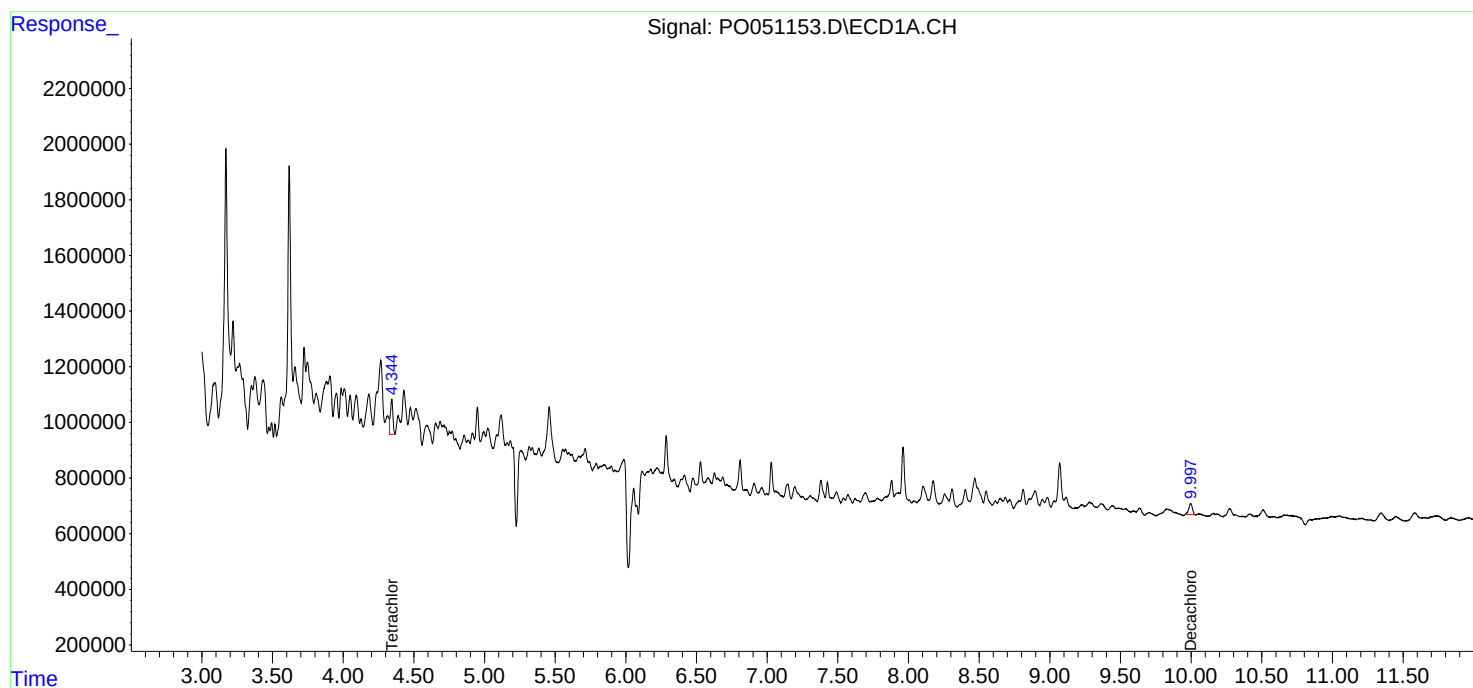

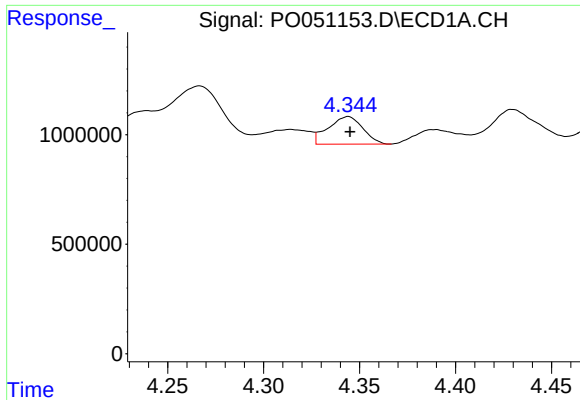


#1 Tetrachloro-m-xylene

R.T.: 4.344 min
Delta R.T.: 0.000 min
Response: 1582547
Conc: 4.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
A366481


Manual Integrations
APPROVED

Sohil
11/7/2018 4:26:53 PM

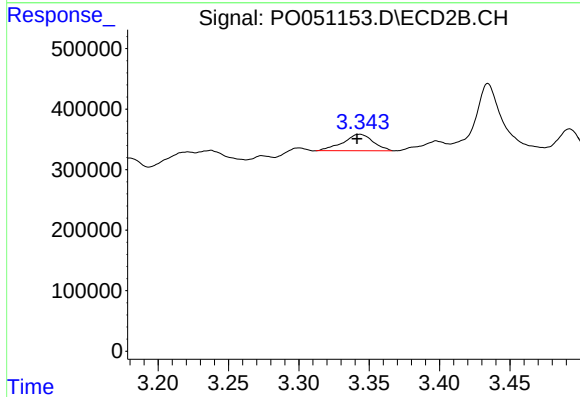


#1 Tetrachloro-m-xylene

R.T.: 3.343 min
Delta R.T.: 0.002 min
Response: 403539
Conc: 1.99 ng/ml m

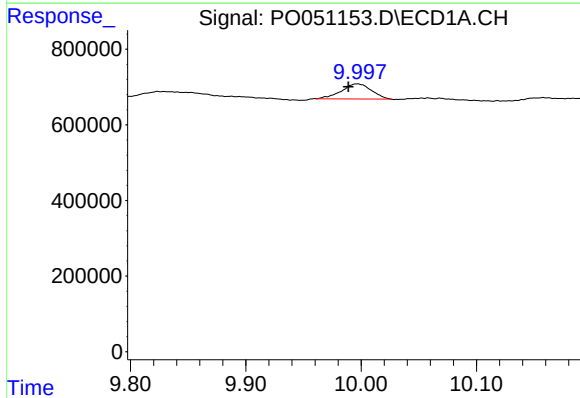

#2 Decachlorobiphenyl

R.T.: 9.997 min
Delta R.T.: 0.008 min
Response: 722063
Conc: 2.43 ng/ml m

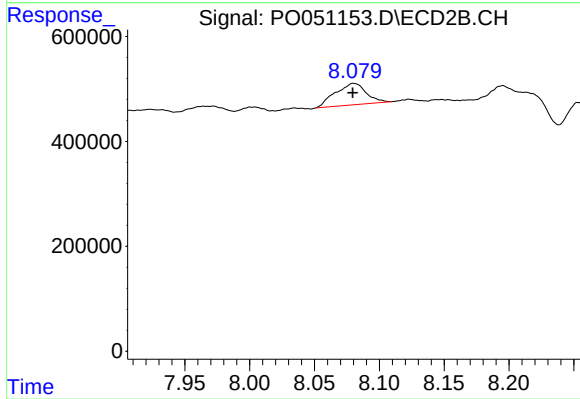

#2 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: 0.000 min
Response: 676756
Conc: 3.06 ng/ml