

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110718\
 Data File : PO051156.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 06 Nov 2018 13:33
 Operator : SM/SJ
 Sample : J5767-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-110118-D

Manual Integrations
 APPROVED

Sohil
 11/7/2018 4:27:00 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 06 14:48:10 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 06 00:37:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.339	5687271	2353505	15.244m	11.609m
2) SA Decachlor...	9.992	8.080	3819110	2053857	12.841m	9.276 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110718\
Data File : PO051156.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Nov 2018 13:33
Operator : SM/SJ
Sample : J5767-07
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CL-02-110118-D


Manual Integrations
APPROVED

Sohil
11/7/2018 4:27:00 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 06 14:48:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 00:37:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

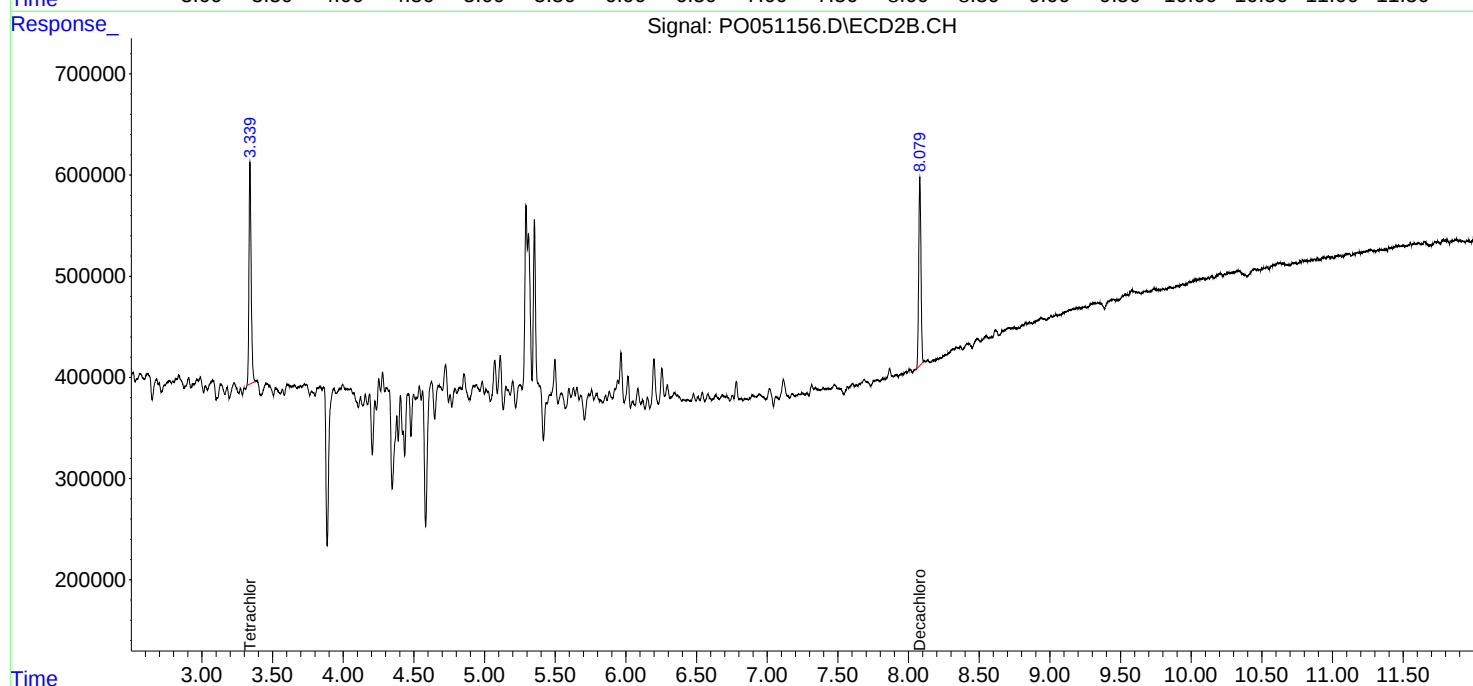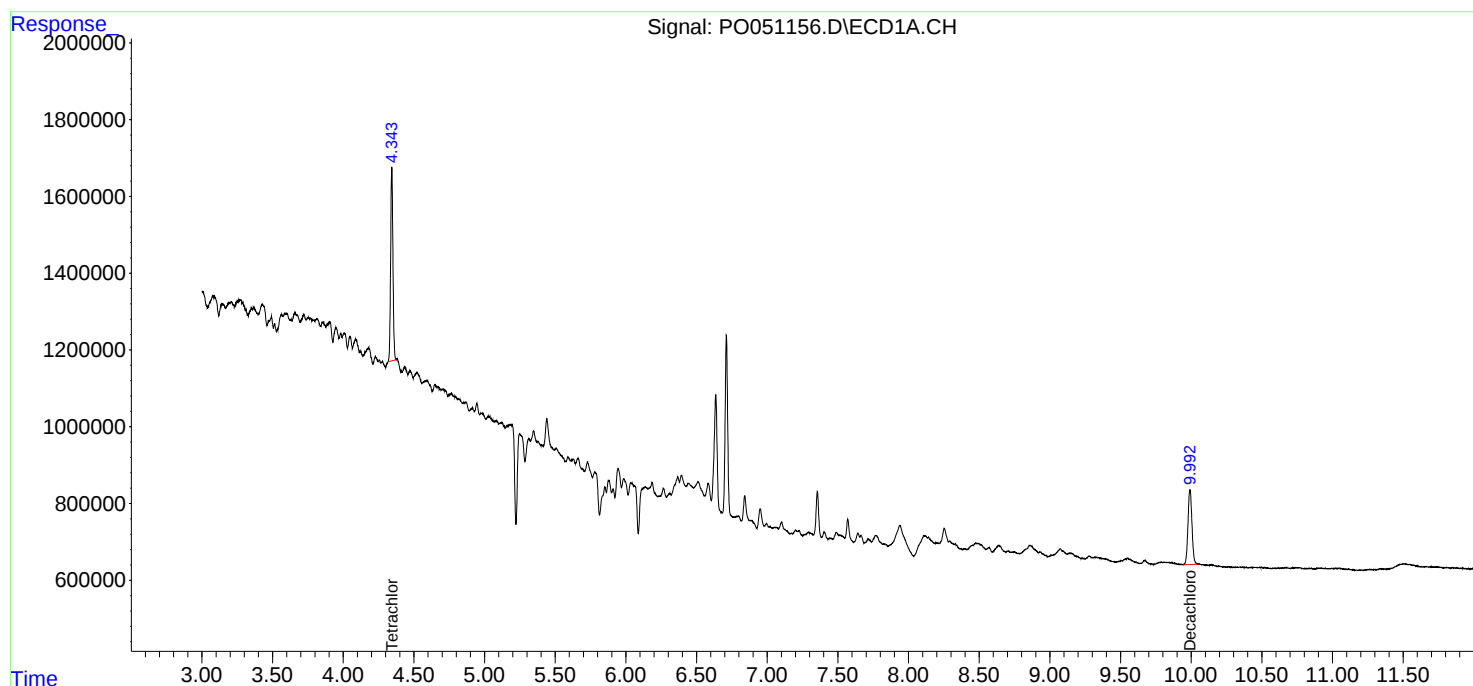

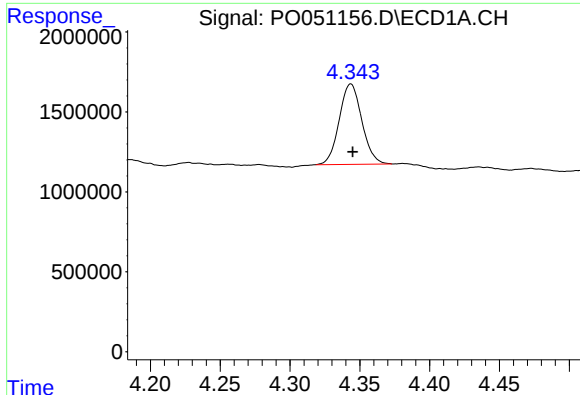


#1 Tetrachloro-m-xylene

R.T.: 4.343 min
Delta R.T.: -0.002 min
Response: 5687271
Conc: 15.24 ng/ml m

Instrument :
ECD_O
ClientSampleId :
CL-02-110118-D


Manual Integrations
APPROVED

Sohil
11/7/2018 4:27:00 PM

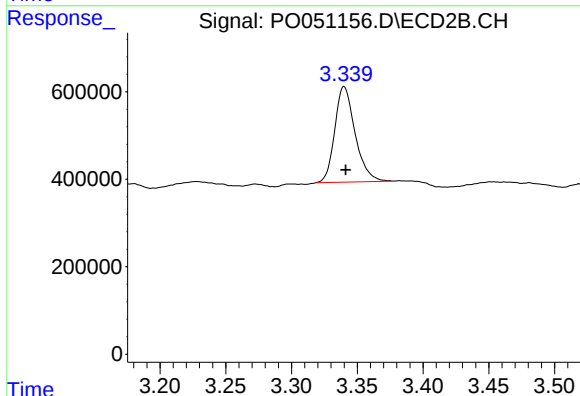


#1 Tetrachloro-m-xylene

R.T.: 3.339 min
Delta R.T.: -0.002 min
Response: 2353505
Conc: 11.61 ng/ml m

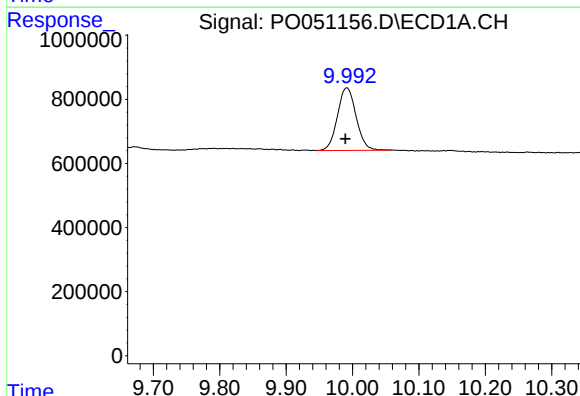

#2 Decachlorobiphenyl

R.T.: 9.992 min
Delta R.T.: 0.003 min
Response: 3819110
Conc: 12.84 ng/ml m

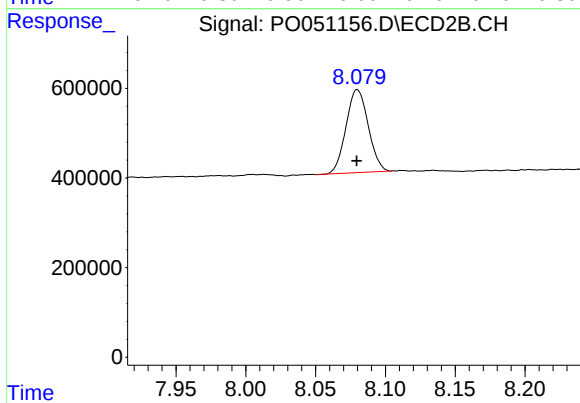

#2 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: 0.000 min
Response: 2053857
Conc: 9.28 ng/ml