

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110718\
Data File : PO051176.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Nov 2018 23:09
Operator : SM/SJ
Sample : J5812-25
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP4-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:06:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 00:37:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.343	3.340	9723318	3686691	26.063	17.870 #
2) SA Decachlor...	9.990	8.078	4087408	2979431	13.840	14.035

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO110718\
Data File : PO051176.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 06 Nov 2018 23:09
Operator : SM/SJ
Sample : J5812-25
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TP4-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 07 08:06:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110518.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 06 00:37:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

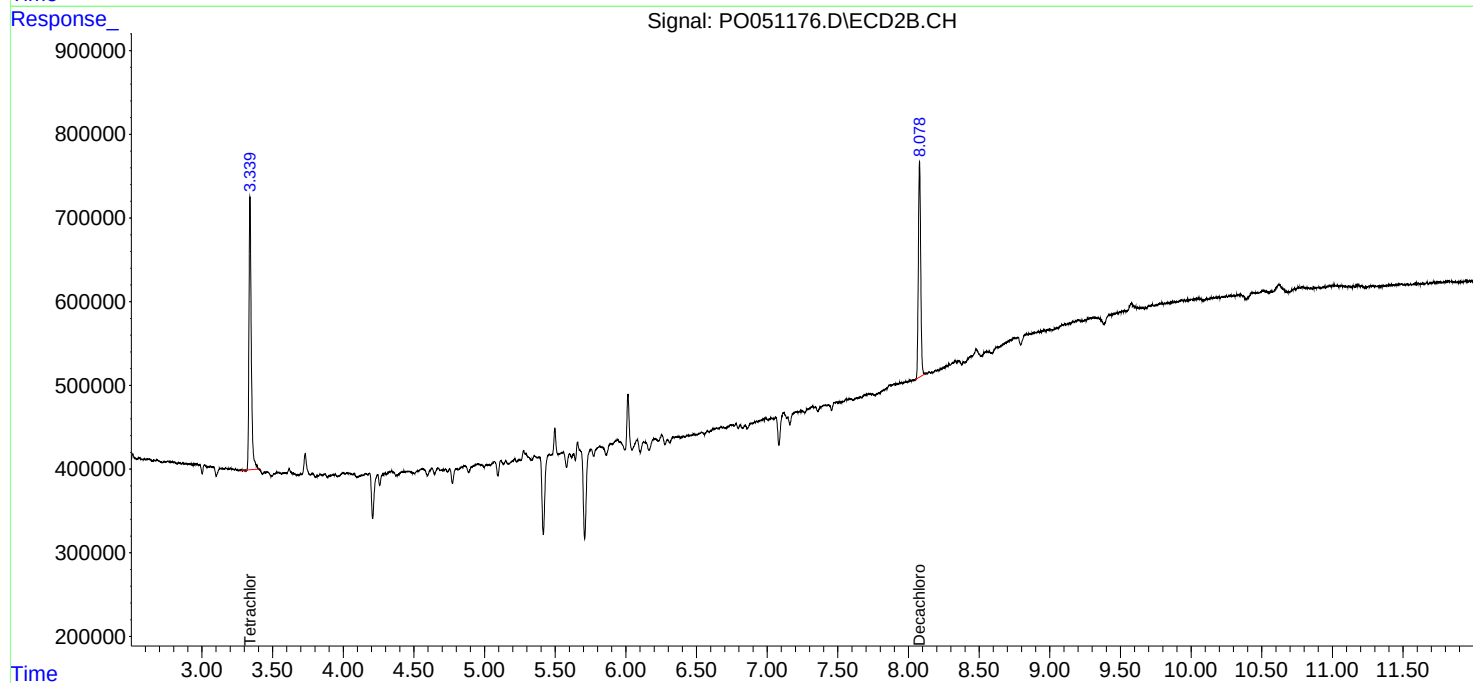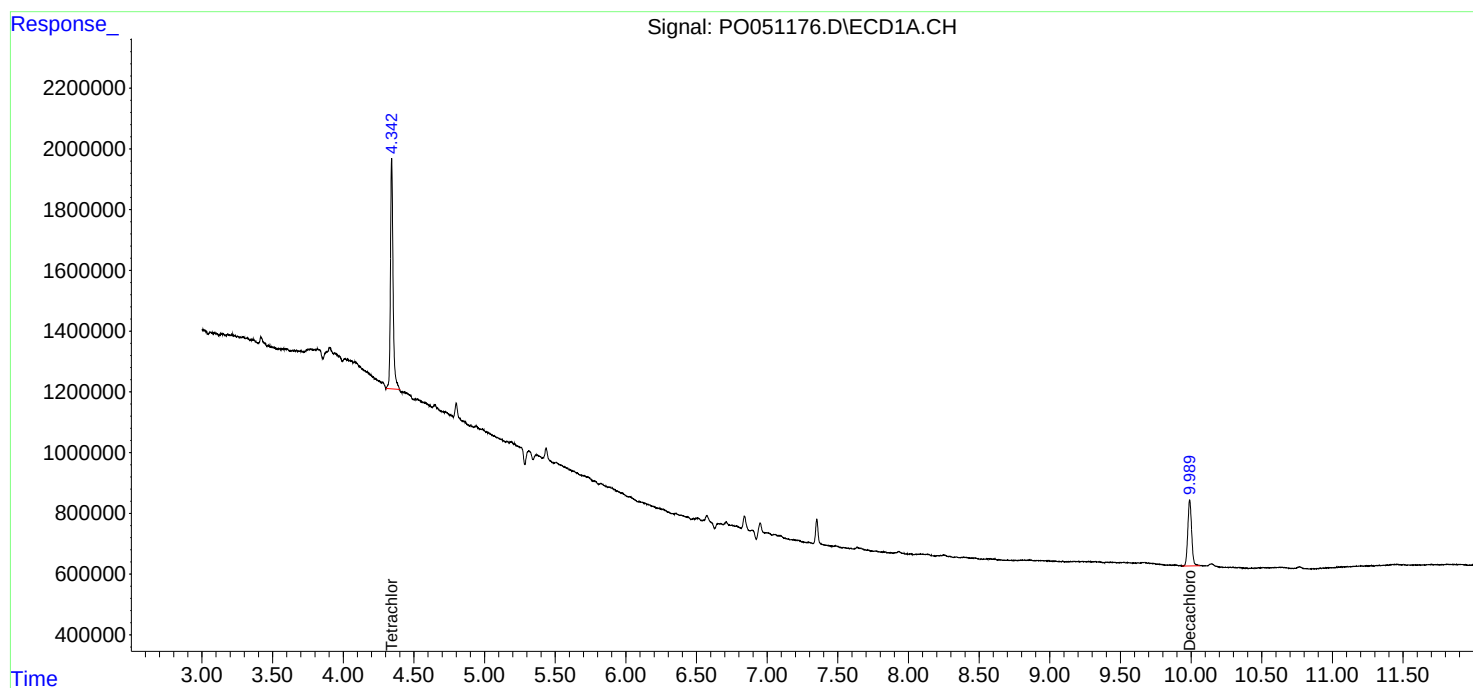


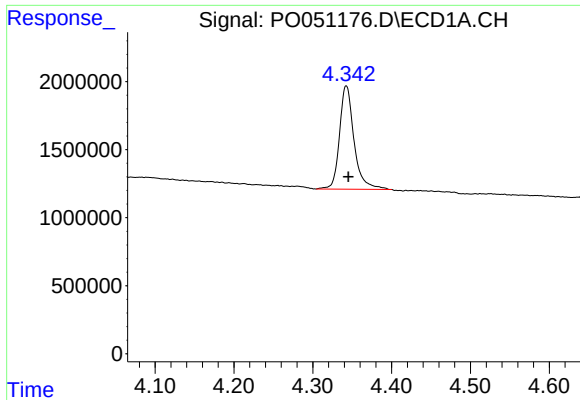

#1 Tetrachloro-m-xylene


R.T.: 4.343 min
Delta R.T.: -0.002 min
Response: 9723318
Conc: 26.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
TP4-A

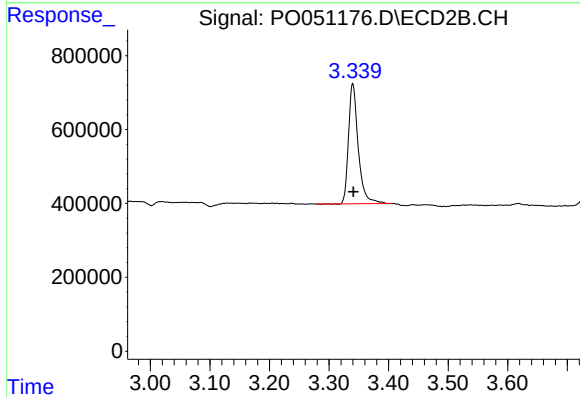


#1 Tetrachloro-m-xylene

R.T.: 3.340 min
Delta R.T.: -0.001 min
Response: 3686691
Conc: 17.87 ng/ml

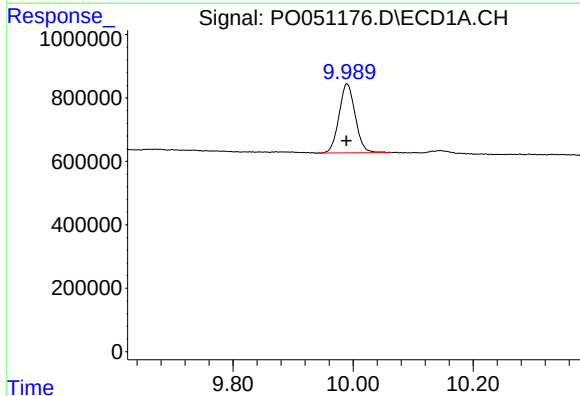

#2 Decachlorobiphenyl

R.T.: 9.990 min
Delta R.T.: 0.000 min
Response: 4087408
Conc: 13.84 ng/ml

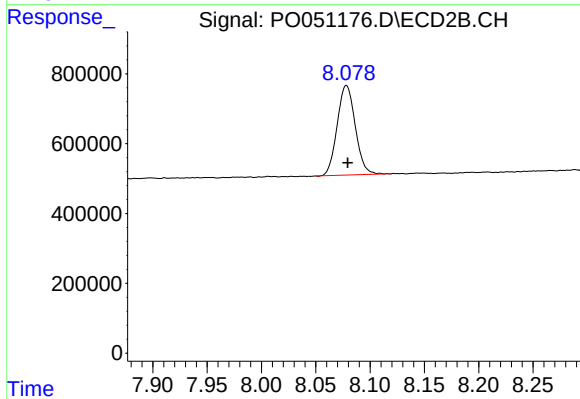

#2 Decachlorobiphenyl

R.T.: 8.078 min
Delta R.T.: -0.001 min
Response: 2979431
Conc: 14.03 ng/ml