

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111218\
 Data File : PO051431.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Nov 2018 00:30
 Operator : SM/SJ
 Sample : PB113884BL
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PB113884BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 06:26:17 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 13 02:51:44 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.329	3.332	13975294	4550456	24.789	20.393
2) SA Decachlor...	9.959	8.059	8569187	5354000	23.093	24.156

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111218\
Data File : PO051431.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2018 00:30
Operator : SM/SJ
Sample : PB113884BL
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PB113884BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 06:26:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO110918.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 13 02:51:44 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

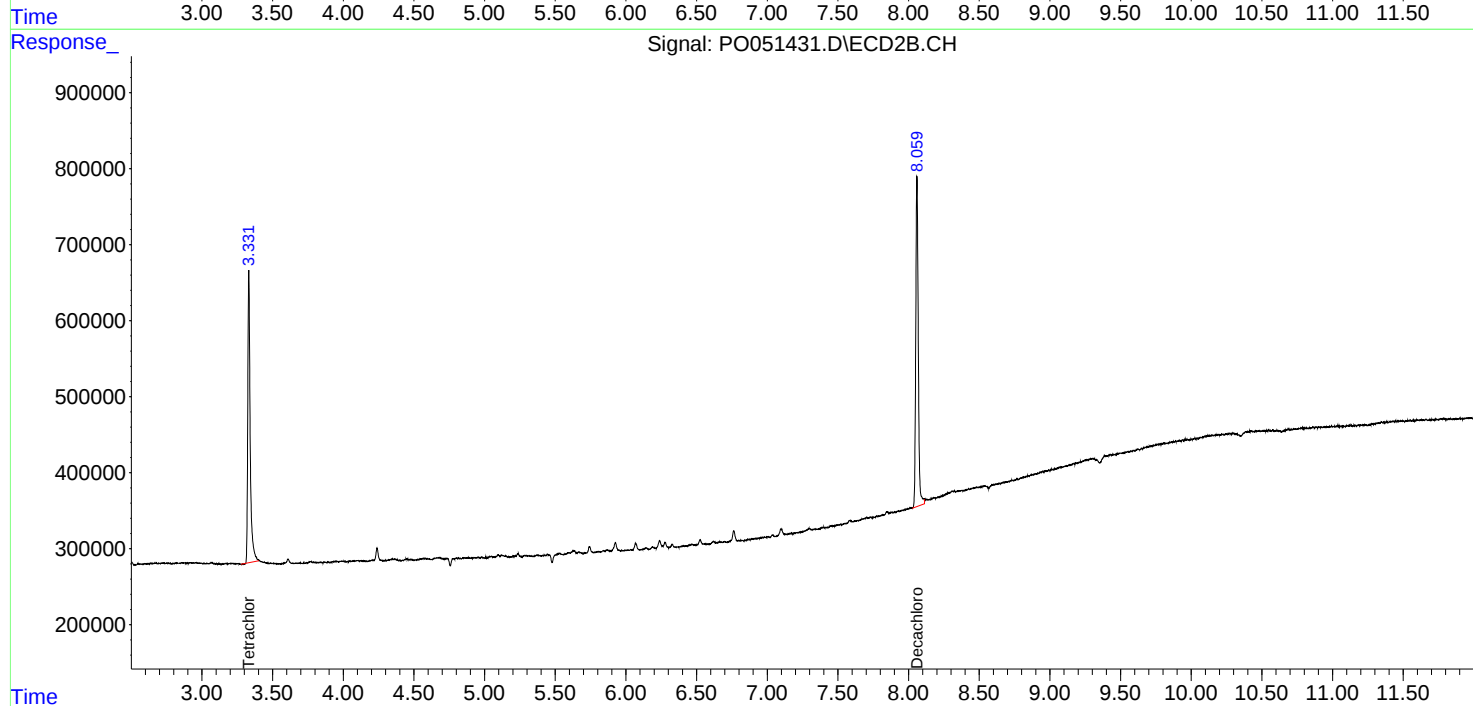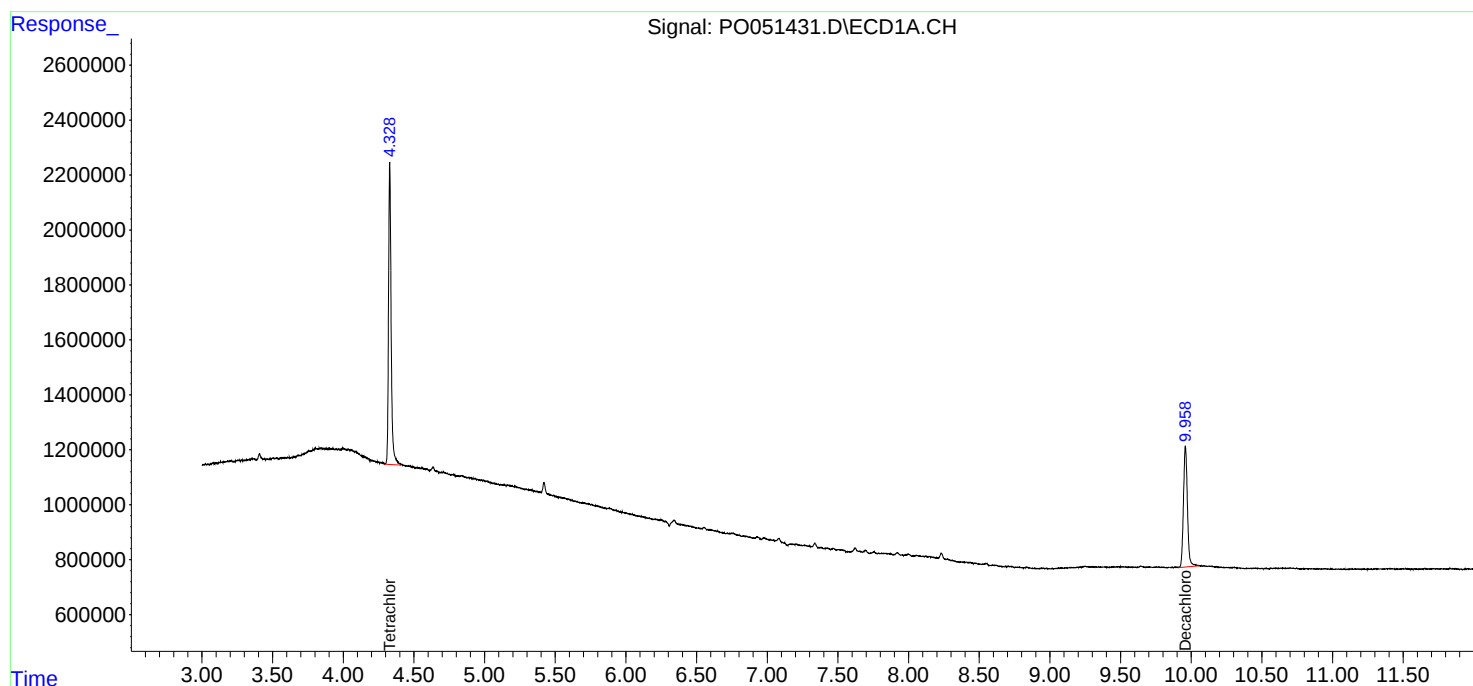


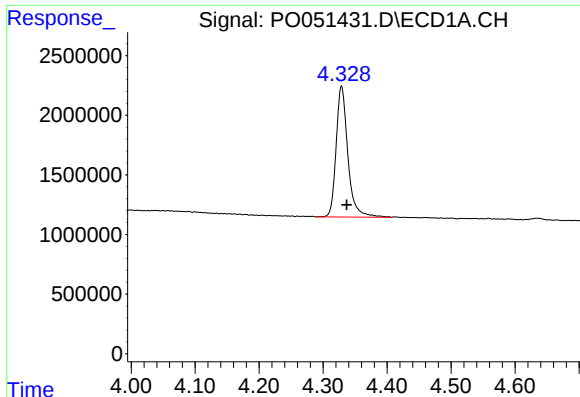

#1 Tetrachloro-m-xylene


R.T.: 4.329 min
Delta R.T.: -0.008 min
Response: 13975294
Conc: 24.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
PB113884BL

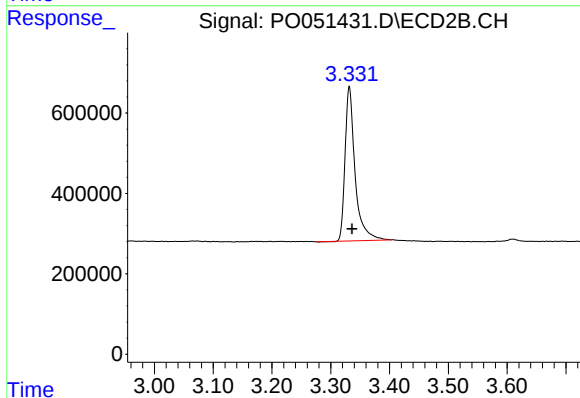


#1 Tetrachloro-m-xylene

R.T.: 3.332 min
Delta R.T.: -0.005 min
Response: 4550456
Conc: 20.39 ng/ml

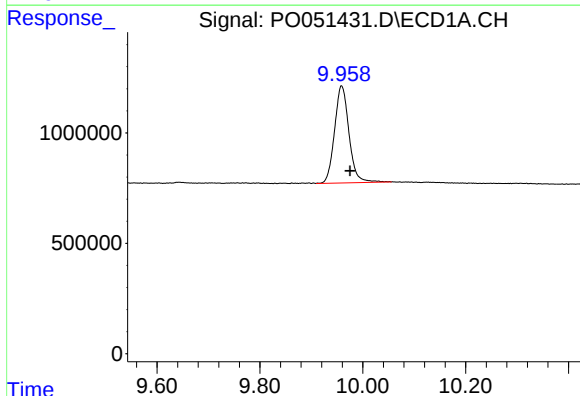

#2 Decachlorobiphenyl

R.T.: 9.959 min
Delta R.T.: -0.017 min
Response: 8569187
Conc: 23.09 ng/ml

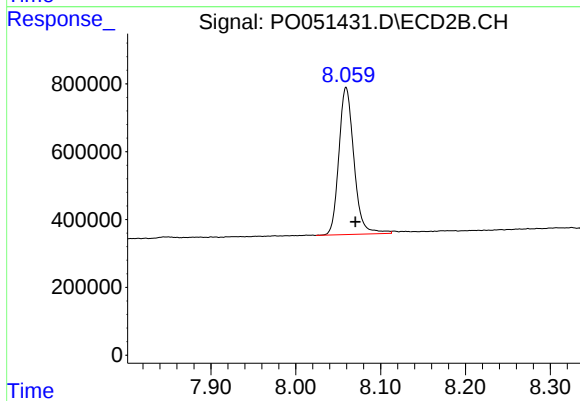

#2 Decachlorobiphenyl

R.T.: 8.059 min
Delta R.T.: -0.011 min
Response: 5354000
Conc: 24.16 ng/ml