

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111719\
 Data File : P0063790.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2019 12:50
 Operator : SM/AJ
 Sample : K5857-03RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-4-1RE

Manual Integrations
 APPROVED

Ankita
 11/18/2019 4:29:08 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:04:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.314	3.567	398123	251967	13.021	11.344m
2)	SA Decachlor...	9.936	8.535	266380	196663	6.555	6.724

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111719\
Data File : PO063790.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2019 12:50
Operator : SM/AJ
Sample : K5857-03RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-4-1RE


Manual Integrations
APPROVED

Ankita
11/18/2019 4:29:08 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:04:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

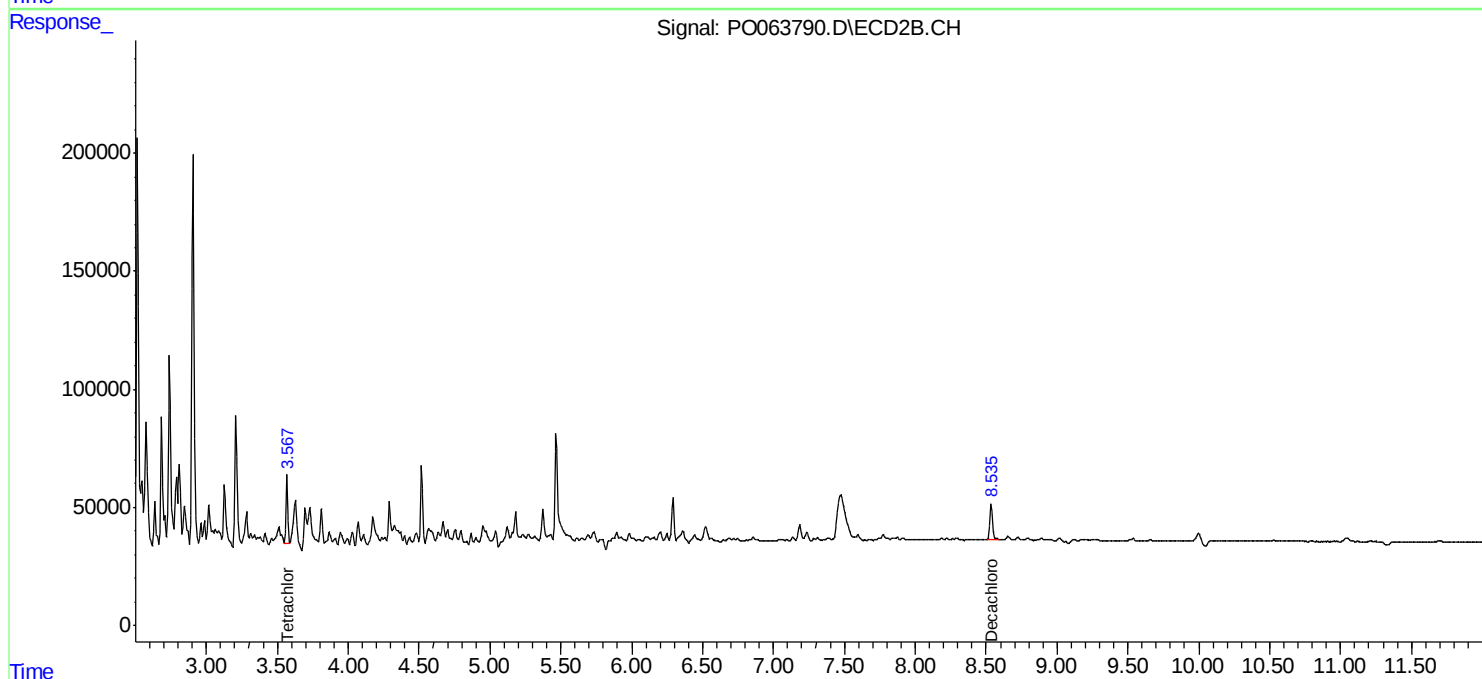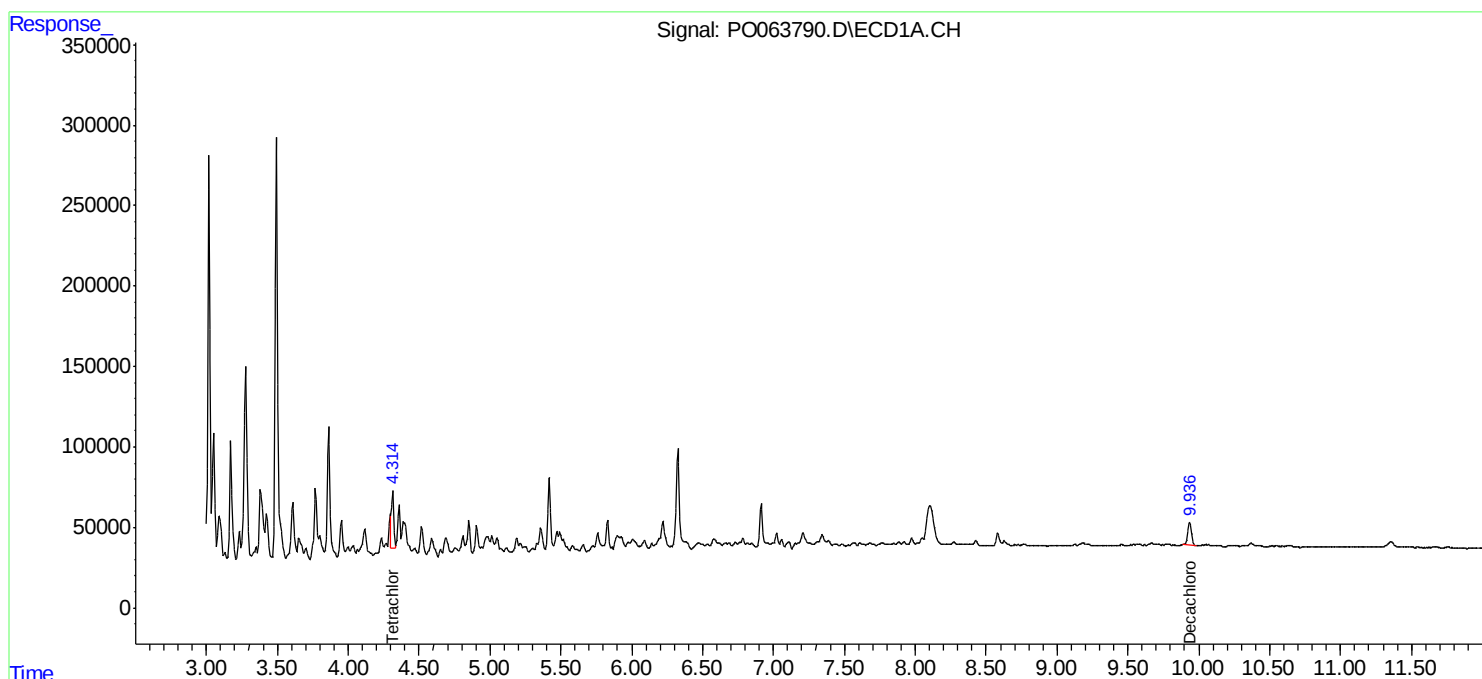

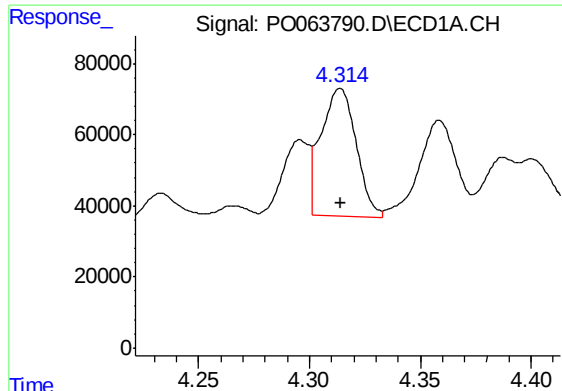


#1 Tetrachloro-m-xylene

R.T.: 4.314 min
Delta R.T.: 0.000 min
Response: 398123
Conc: 13.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-4-1RE


Manual Integrations
APPROVED

Ankita
11/18/2019 4:29:08 PM

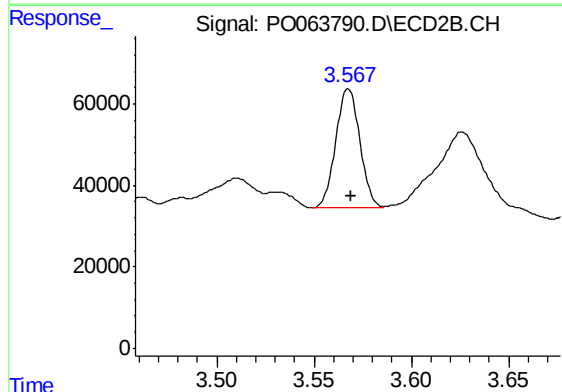


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: -0.001 min
Response: 251967
Conc: 11.34 ng/ml m

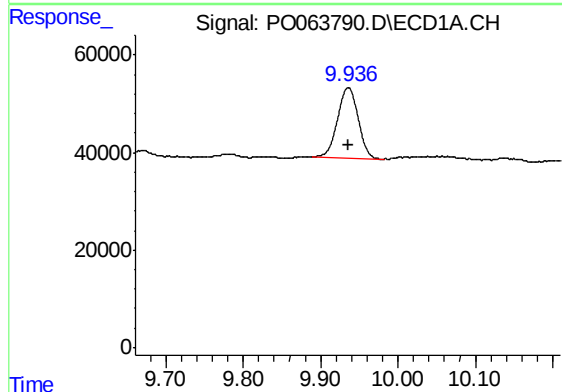

#2 Decachlorobiphenyl

R.T.: 9.936 min
Delta R.T.: 0.000 min
Response: 266380
Conc: 6.56 ng/ml

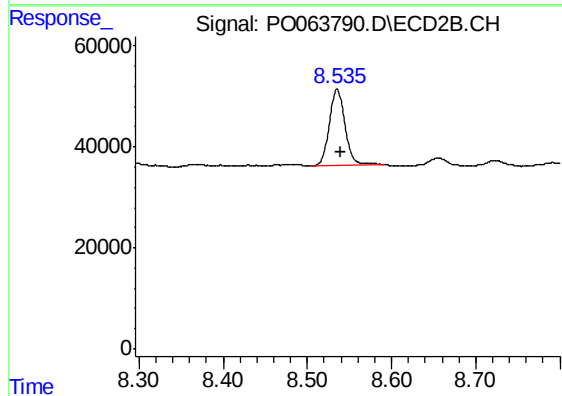

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.004 min
Response: 196663
Conc: 6.72 ng/ml