

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111719\
Data File : P0063803.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2019 16:59
Operator : SM/AJ
Sample : K5840-03RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PHIPPS-BH-NE-01RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:11:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.315	3.568	908382	666687	29.710	30.016
2) SA Decachlor...	9.937	8.536	755105	532726	18.583	18.215

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111719\
Data File : PO063803.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2019 16:59
Operator : SM/AJ
Sample : K5840-03RE
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PHIPPS-BH-NE-01RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:11:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

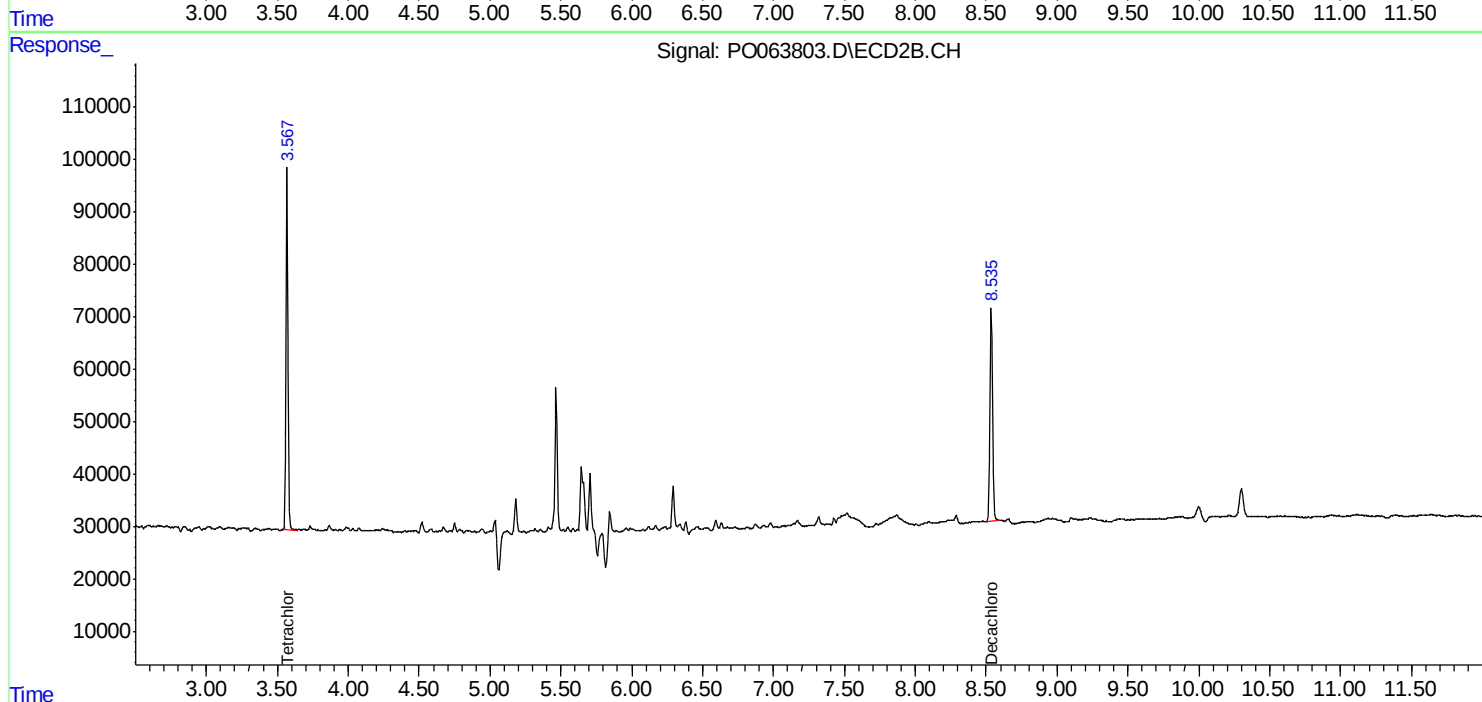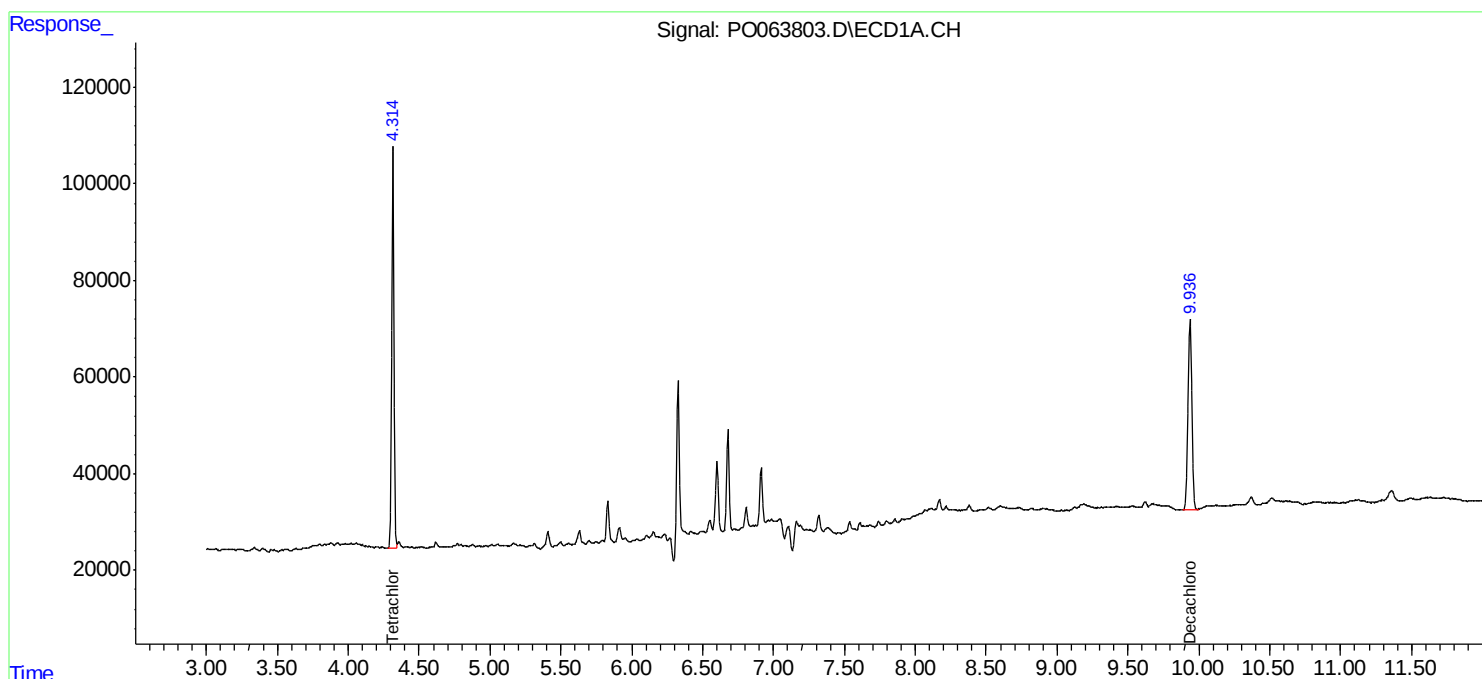


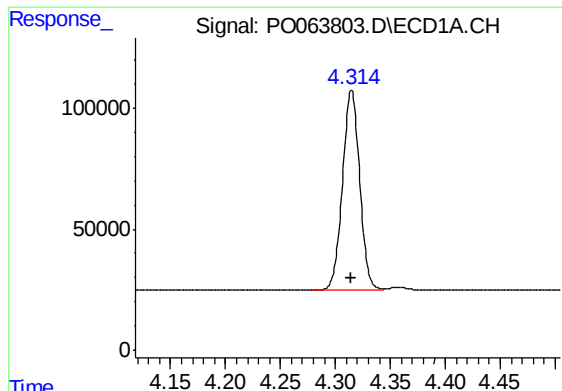

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.000 min
Response: 908382
Conc: 29.71 ng/ml

Instrument :
ECD_O
ClientSampleId :
PHIPPS-BH-NE-01RE

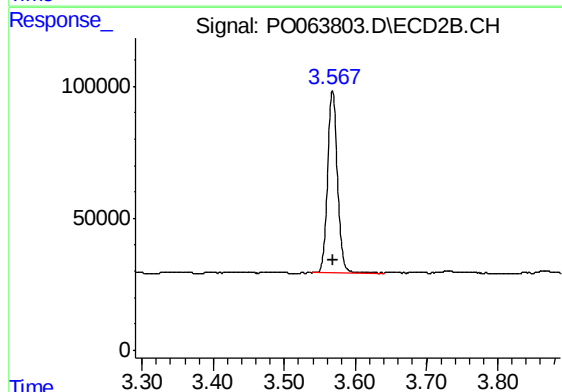


#1 Tetrachloro-m-xylene

R.T.: 3.568 min
Delta R.T.: 0.000 min
Response: 666687
Conc: 30.02 ng/ml

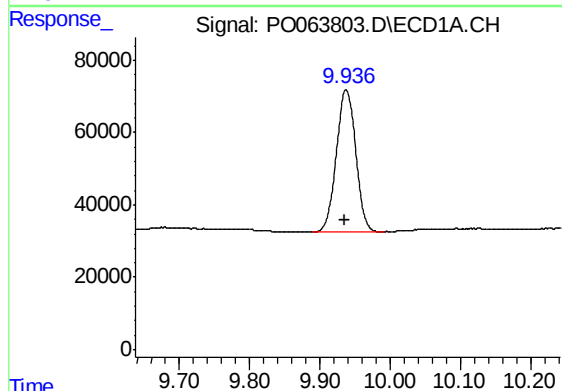

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: 0.001 min
Response: 755105
Conc: 18.58 ng/ml

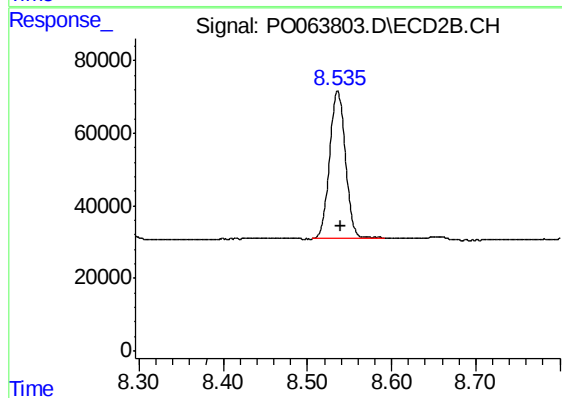

#2 Decachlorobiphenyl

R.T.: 8.536 min
Delta R.T.: -0.004 min
Response: 532726
Conc: 18.21 ng/ml