

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO111719\
 Data File : P0063807.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2019 18:05
 Operator : SM/AJ
 Sample : K5839-01RE
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PHIPPS-BH-NW-01RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:13:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO111419.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 15 01:29:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.315	3.569	934897	702493	30.577	31.628
2) SA Decachlor...	9.938	8.537	730590	495803	17.979	16.952

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0111719\
Data File : P0063807.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2019 18:05
Operator : SM/AJ
Sample : K5839-01RE
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PHIPPS-BH-NW-01RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:13:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0111419.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 15 01:29:03 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

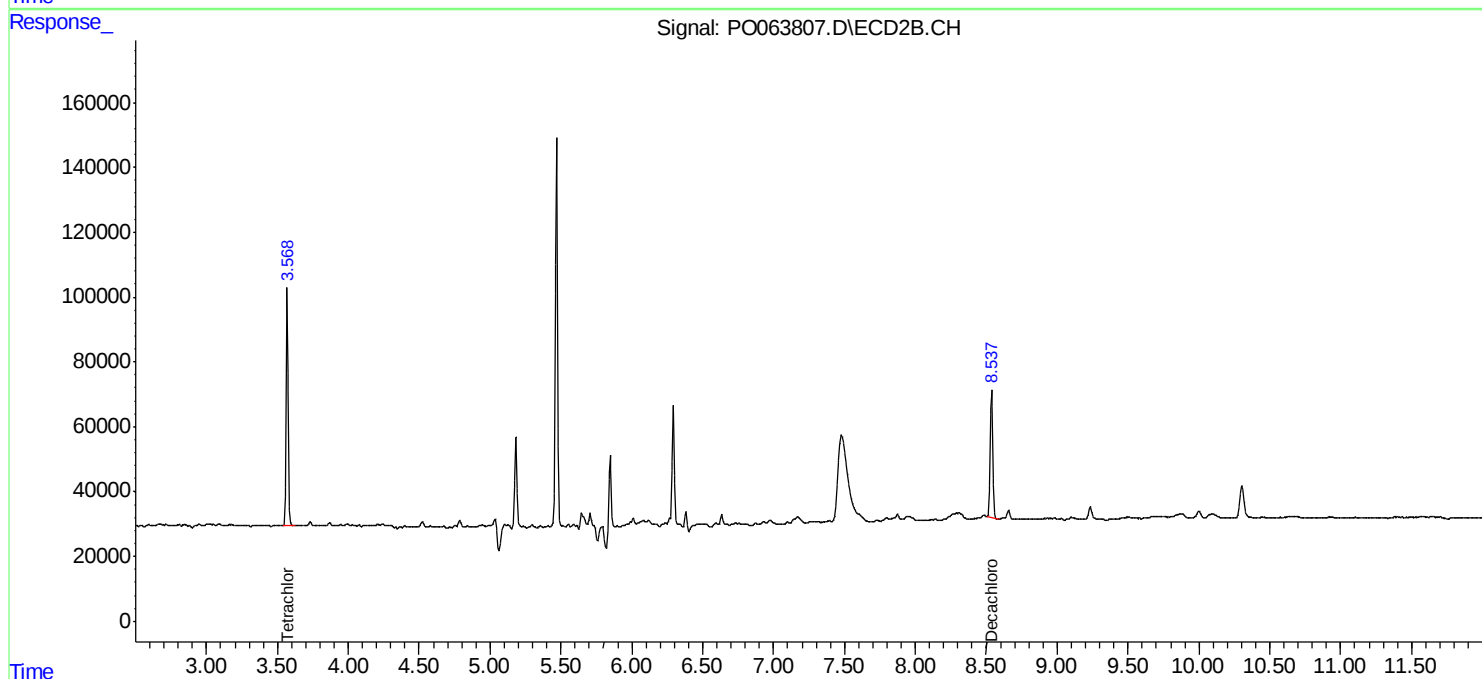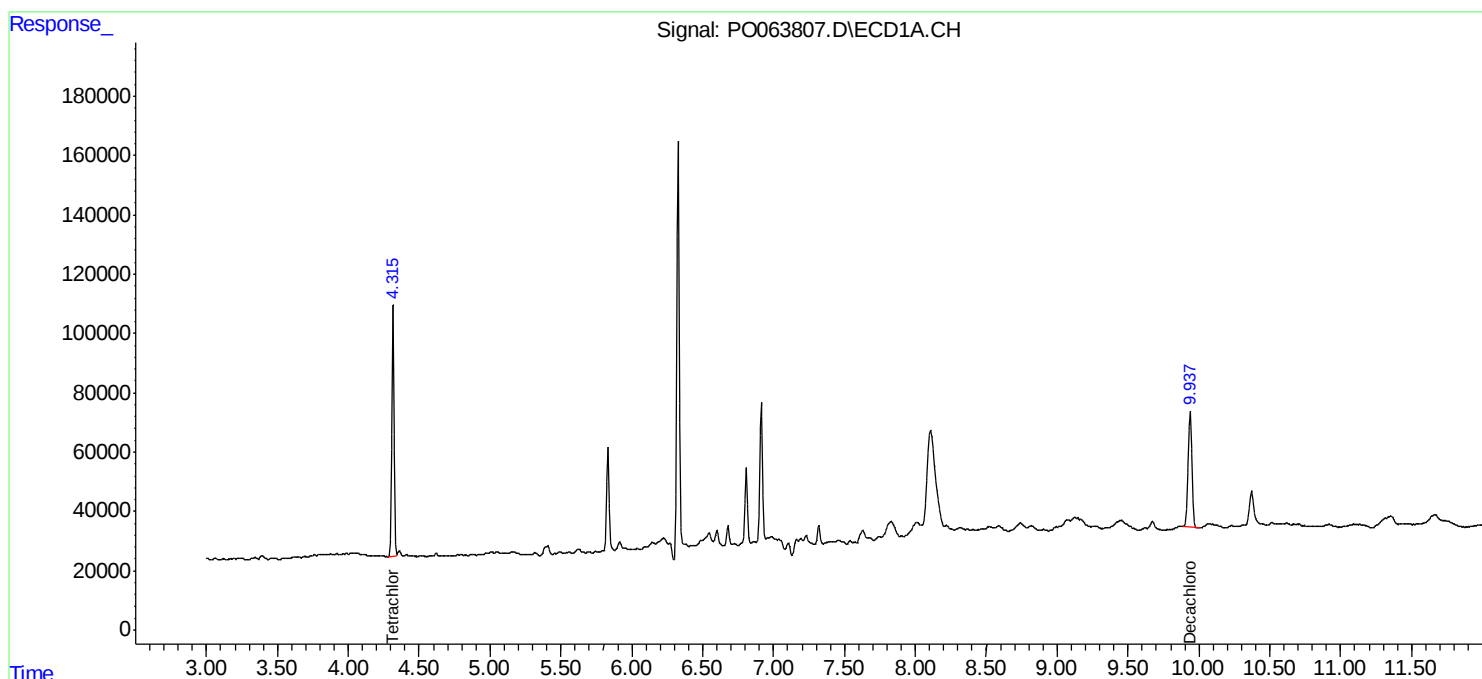


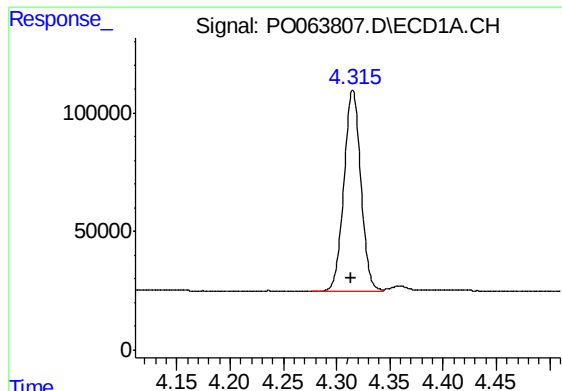

#1 Tetrachloro-m-xylene


R.T.: 4.315 min
Delta R.T.: 0.001 min
Response: 934897
Conc: 30.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
PHIPPS-BH-NW-01RE

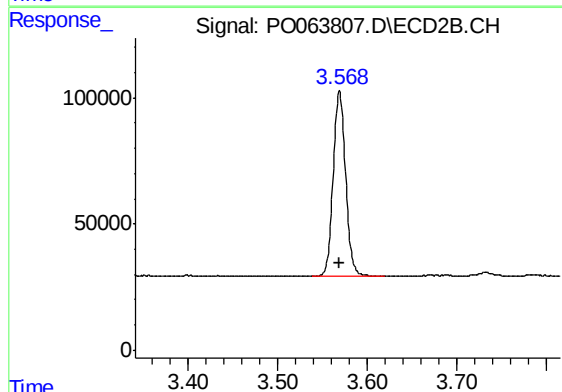


#1 Tetrachloro-m-xylene

R.T.: 3.569 min
Delta R.T.: 0.000 min
Response: 702493
Conc: 31.63 ng/ml

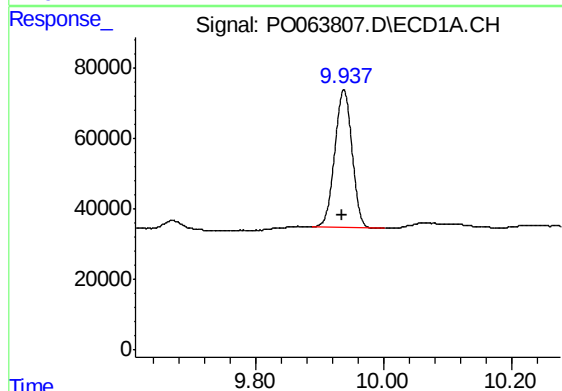

#2 Decachlorobiphenyl

R.T.: 9.938 min
Delta R.T.: 0.002 min
Response: 730590
Conc: 17.98 ng/ml

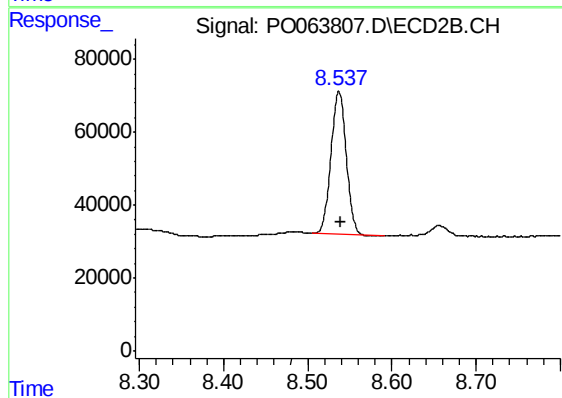

#2 Decachlorobiphenyl

R.T.: 8.537 min
Delta R.T.: -0.002 min
Response: 495803
Conc: 16.95 ng/ml