

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112018\
 Data File : P0051645.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2018 14:37
 Operator : SM/SJ
 Sample : J5970-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 FK-GF-02-028-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 03:03:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 21 00:55:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.330	3.322	12911262	3829473	17.151	15.999
2)	SA Decachlor...	9.958	8.049	5951500	2873505	12.830	13.293

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112018\
Data File : PO051645.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2018 14:37
Operator : SM/SJ
Sample : J5970-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-028-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 03:03:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 21 00:55:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

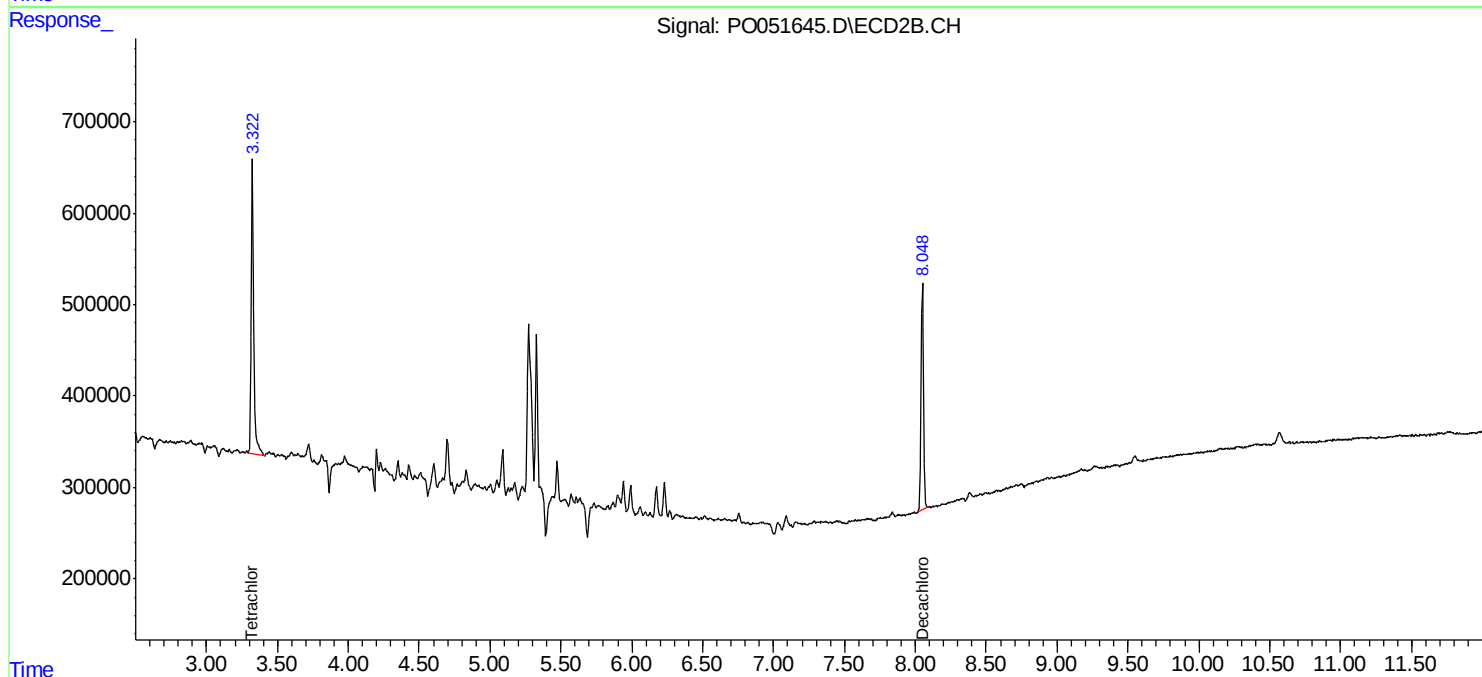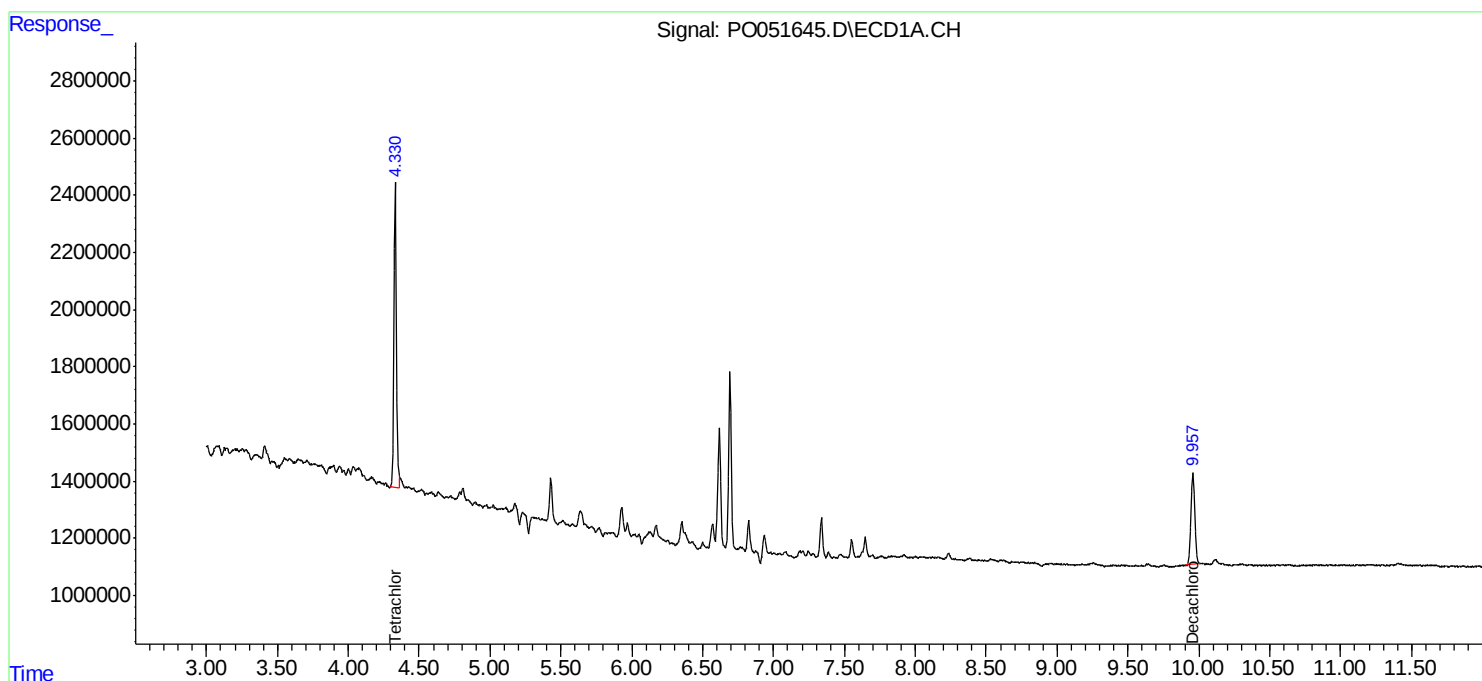


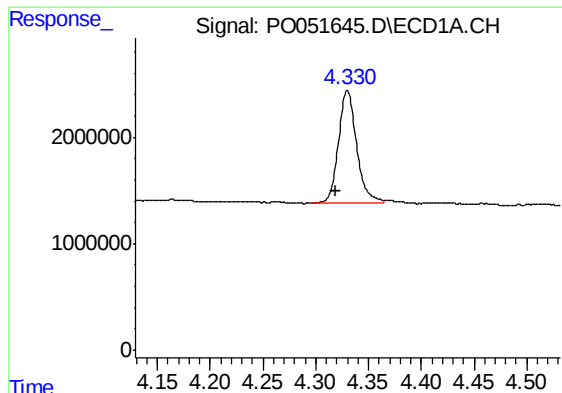

#1 Tetrachloro-m-xylene


R.T.: 4.330 min
Delta R.T.: 0.011 min
Response: 12911262
Conc: 17.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
FK-GF-02-028-A

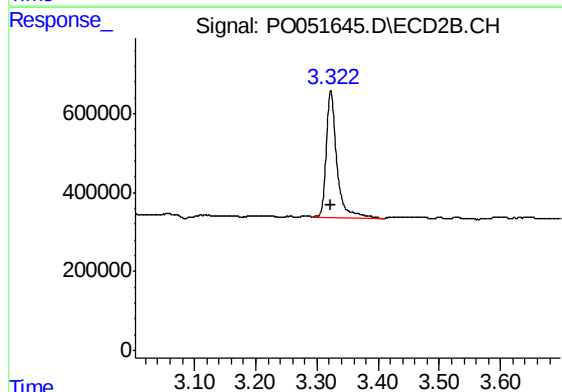


#1 Tetrachloro-m-xylene

R.T.: 3.322 min
Delta R.T.: 0.000 min
Response: 3829473
Conc: 16.00 ng/ml

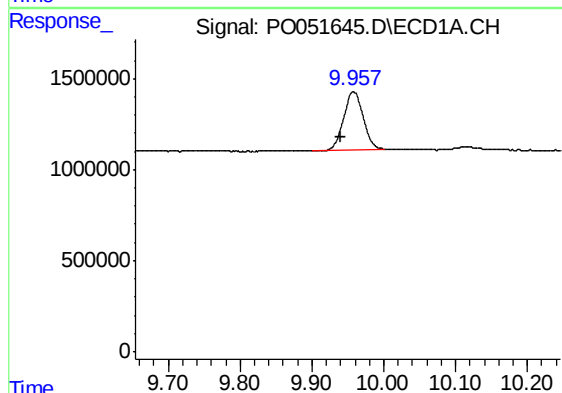

#2 Decachlorobiphenyl

R.T.: 9.958 min
Delta R.T.: 0.017 min
Response: 5951500
Conc: 12.83 ng/ml

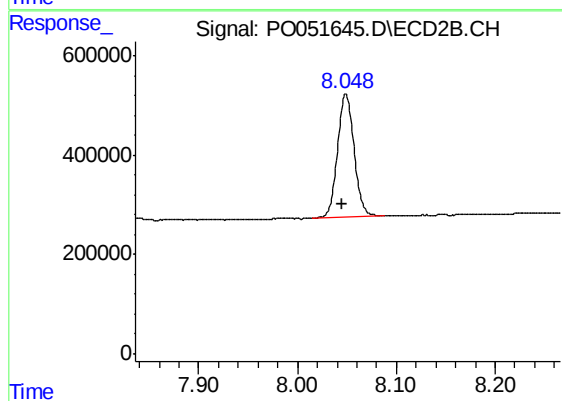

#2 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.004 min
Response: 2873505
Conc: 13.29 ng/ml