

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112018\
 Data File : P0051655.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 20 Nov 2018 17:29
 Operator : SM/SJ
 Sample : J5981-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DTW-01(6-10)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 03:07:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 21 00:55:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.317	3.321	11449806	3558564	15.210	14.867
2)	SA Decachlor...	9.937	8.044	7369473	3355353	15.886	15.522

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112018\
Data File : PO051655.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 20 Nov 2018 17:29
Operator : SM/SJ
Sample : J5981-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
DTW-01(6-10)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 03:07:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 21 00:55:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

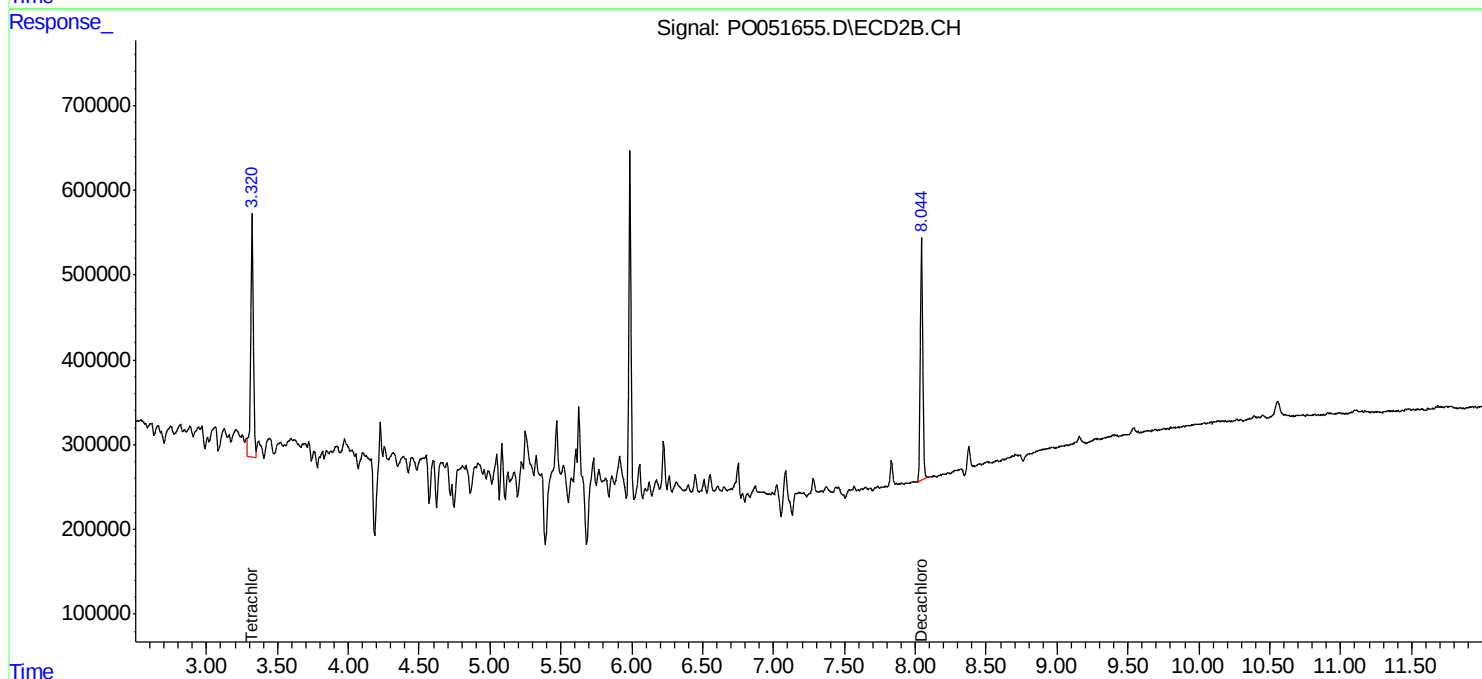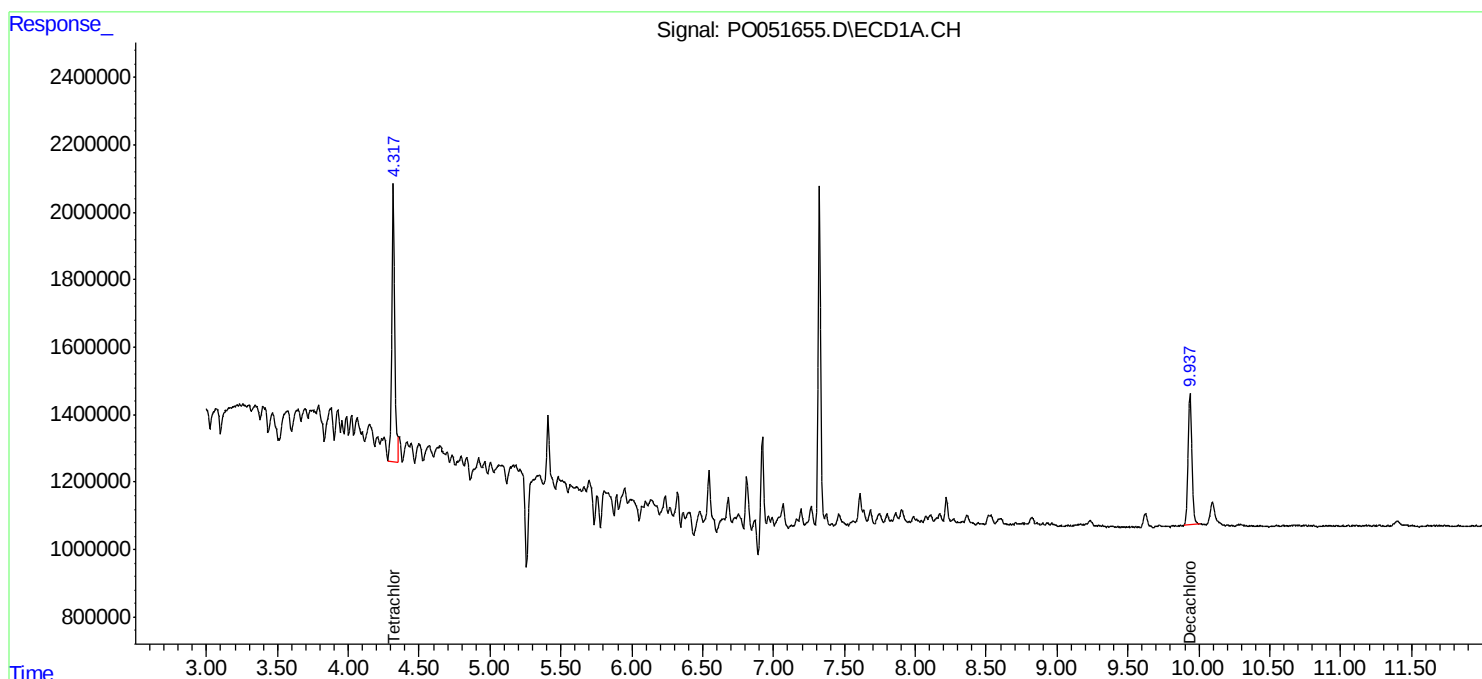


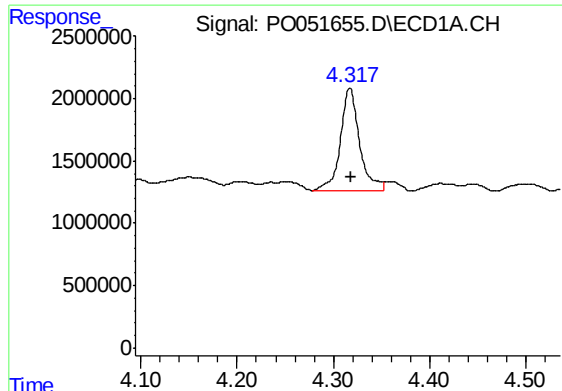

#1 Tetrachloro-m-xylene


R.T.: 4.317 min
Delta R.T.: -0.002 min
Response: 11449806
Conc: 15.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
DTW-01(6-10)

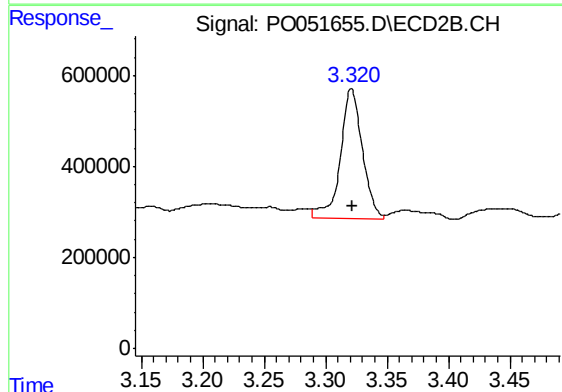


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: -0.001 min
Response: 3558564
Conc: 14.87 ng/ml

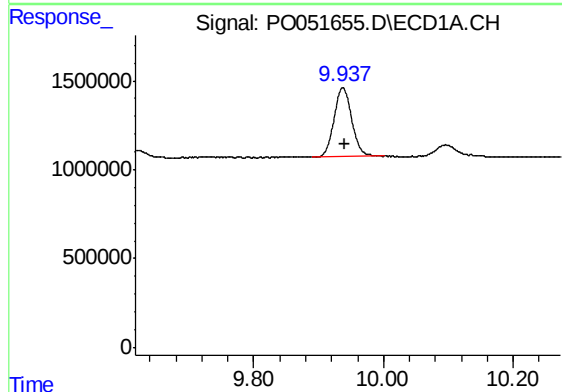

#2 Decachlorobiphenyl

R.T.: 9.937 min
Delta R.T.: -0.003 min
Response: 7369473
Conc: 15.89 ng/ml

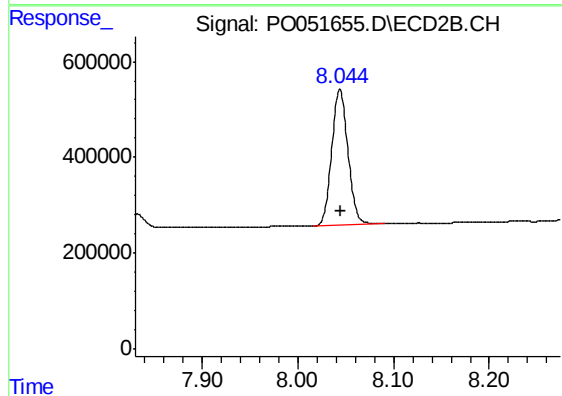

#2 Decachlorobiphenyl

R.T.: 8.044 min
Delta R.T.: -0.001 min
Response: 3355353
Conc: 15.52 ng/ml