

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112018\
 Data File : P0051688.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 21 Nov 2018 3:22
 Operator : SM/SJ
 Sample : J6006-03
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 RS-CON-WALL-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 21 07:08:35 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 21 00:55:28 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.317	3.321	17411218	4831333	23.129	20.184
2) SA Decachlor...	9.935	8.041	27362168	9515470	58.985	44.018 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112018\
Data File : PO051688.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 21 Nov 2018 3:22
Operator : SM/SJ
Sample : J6006-03
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
RS-CON-WALL-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 21 07:08:35 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112018.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 21 00:55:28 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

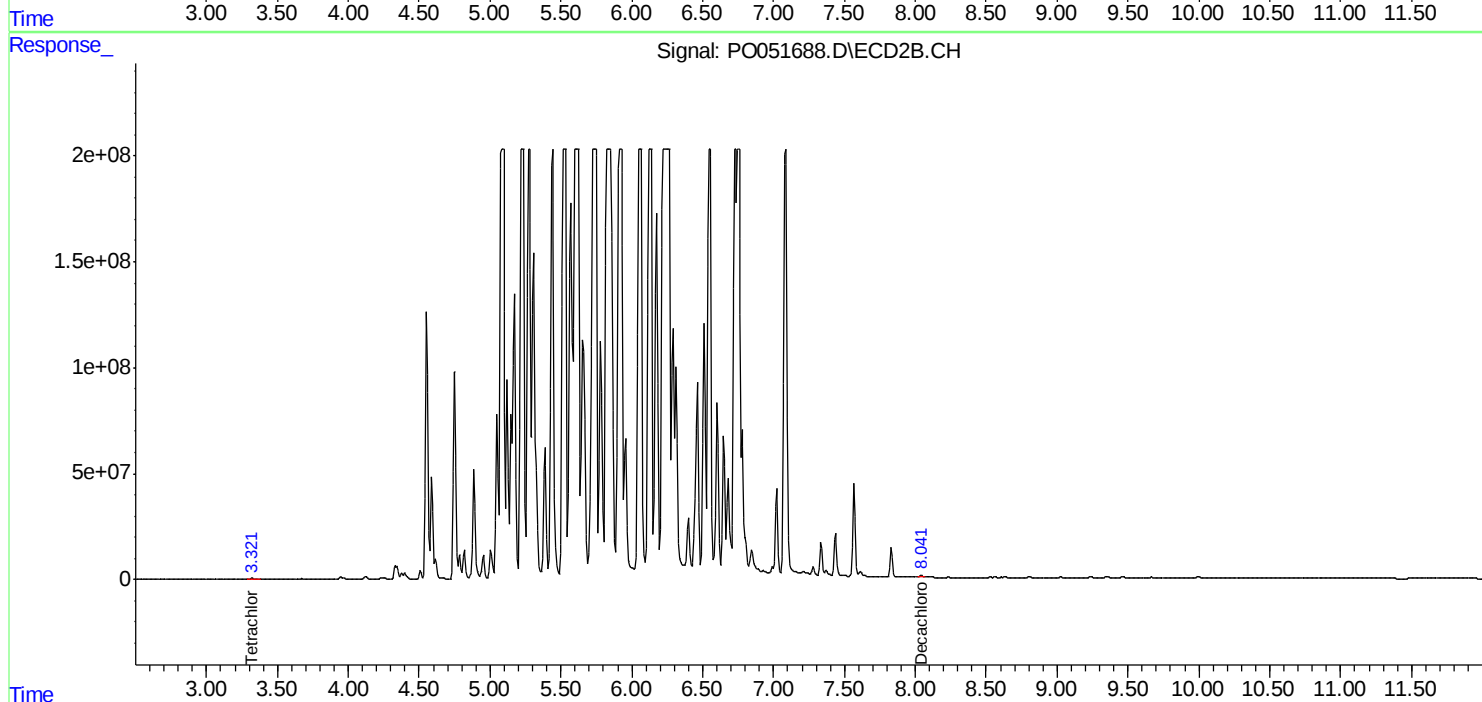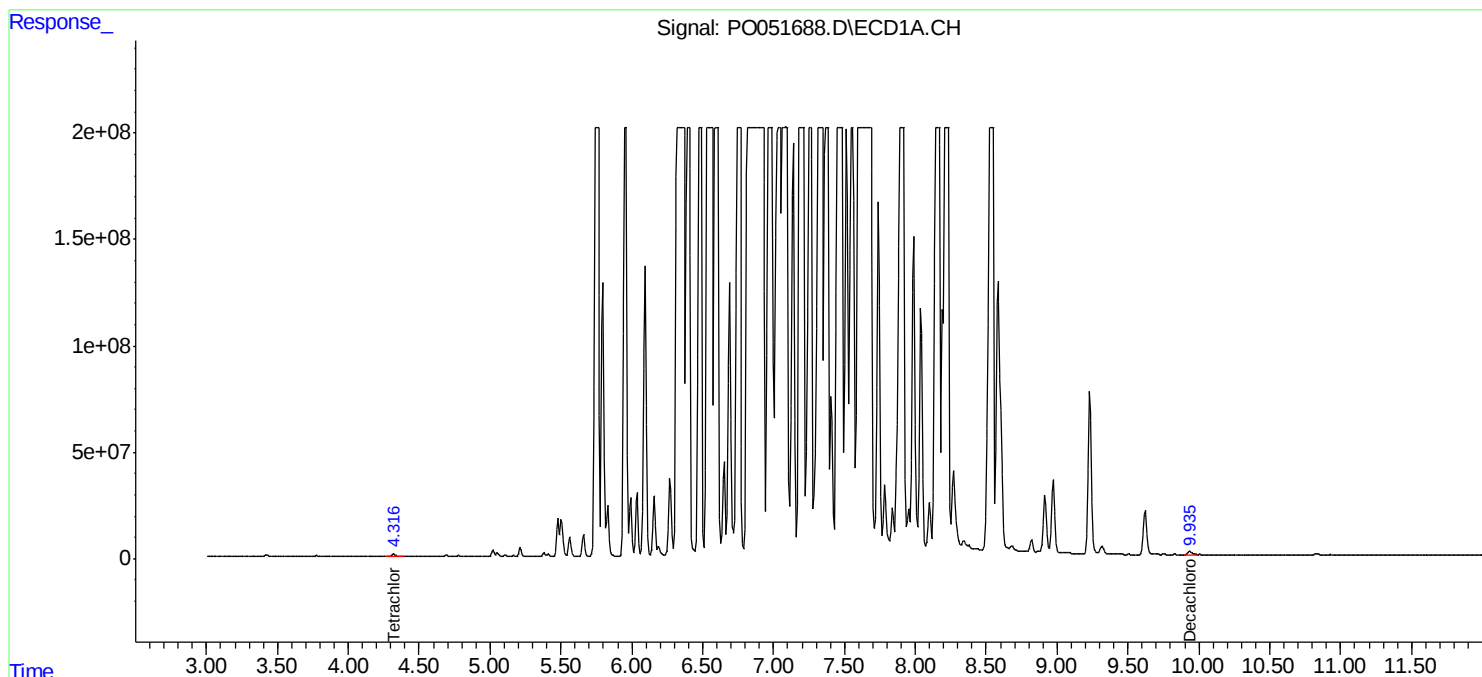


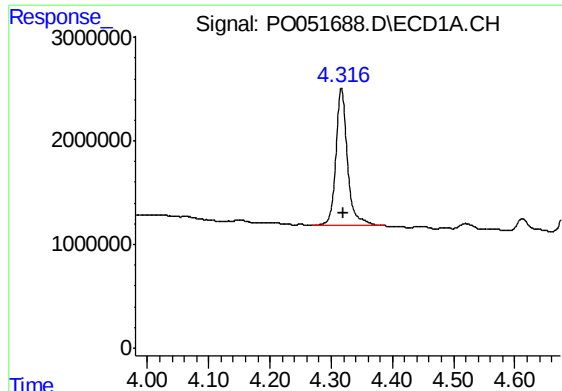

#1 Tetrachloro-m-xylene


R.T.: 4.317 min
Delta R.T.: -0.002 min
Response: 17411218
Conc: 23.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
RS-CON-WALL-2

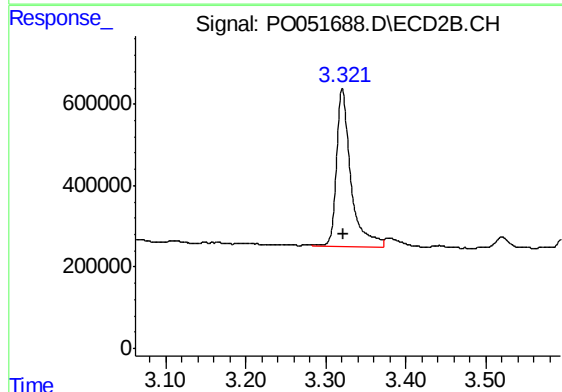


#1 Tetrachloro-m-xylene

R.T.: 3.321 min
Delta R.T.: 0.000 min
Response: 4831333
Conc: 20.18 ng/ml

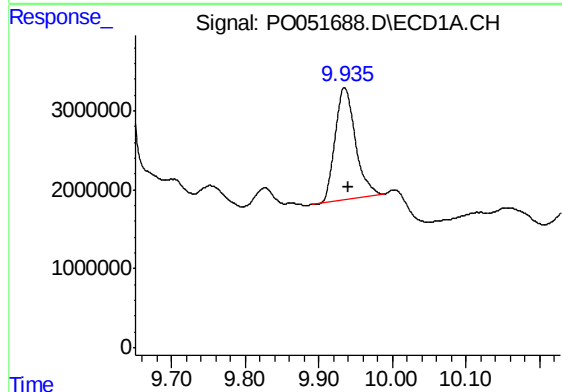

#2 Decachlorobiphenyl

R.T.: 9.935 min
Delta R.T.: -0.005 min
Response: 27362168
Conc: 58.98 ng/ml

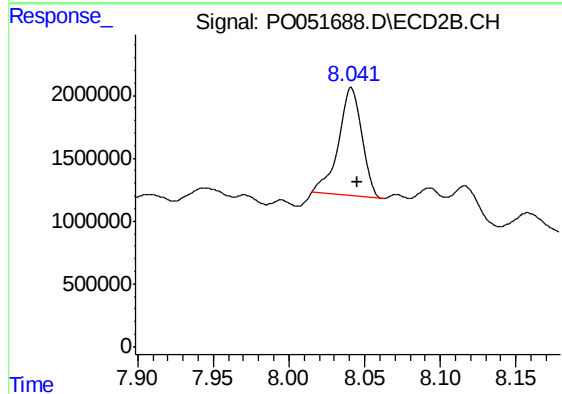

#2 Decachlorobiphenyl

R.T.: 8.041 min
Delta R.T.: -0.004 min
Response: 9515470
Conc: 44.02 ng/ml