

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112818\
 Data File : P0051901.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Nov 2018 13:18
 Operator : SM/SJ
 Sample : J6003-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 NON-UST-03R-A

Manual Integrations
 APPROVED

mohammad
 11/29/2018 2:24:31 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 08:37:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.303	3.311	7981039	2471726	12.234	10.469
2)	SA Decachlor...	9.910	8.025	7148487	3278736	17.143m	16.572

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112818\
Data File : PO051901.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Nov 2018 13:18
Operator : SM/SJ
Sample : J6003-03
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
NON-UST-03R-A


Manual Integrations
APPROVED

mohammad
11/29/2018 2:24:31 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 08:37:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

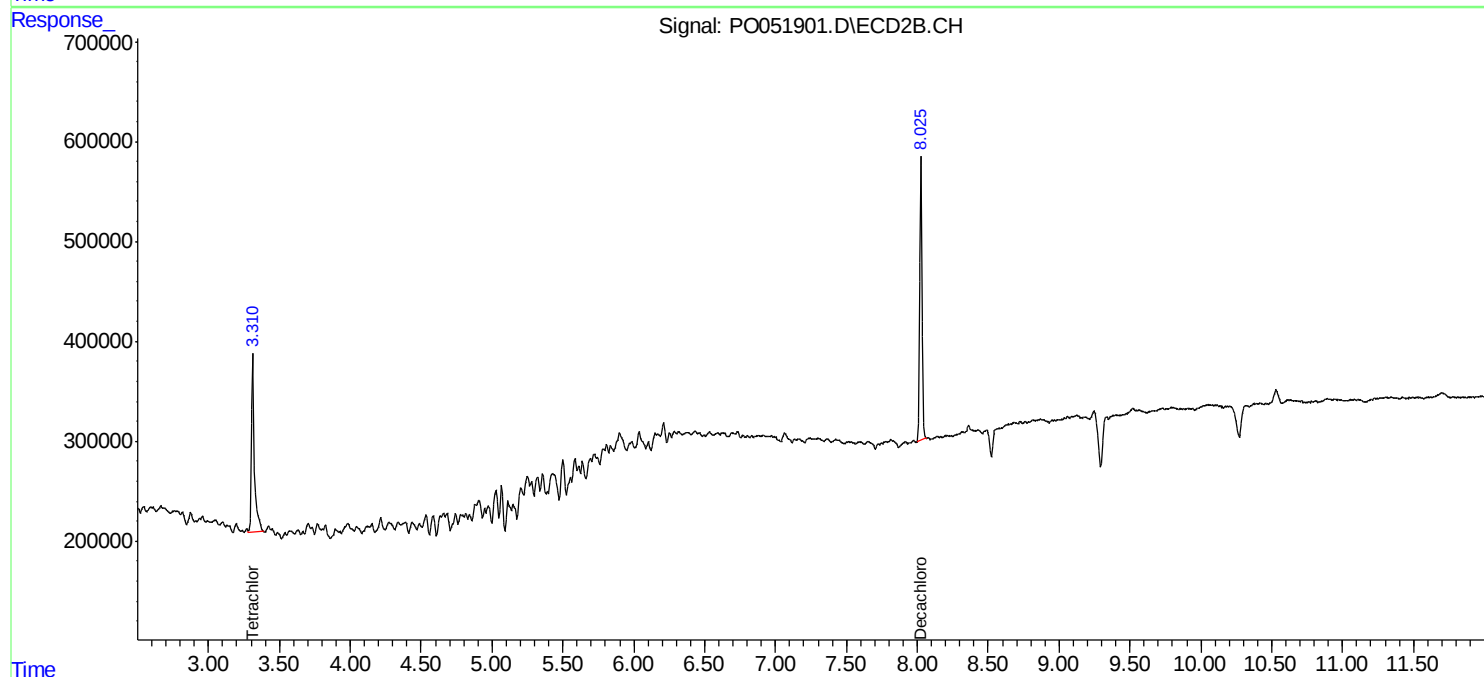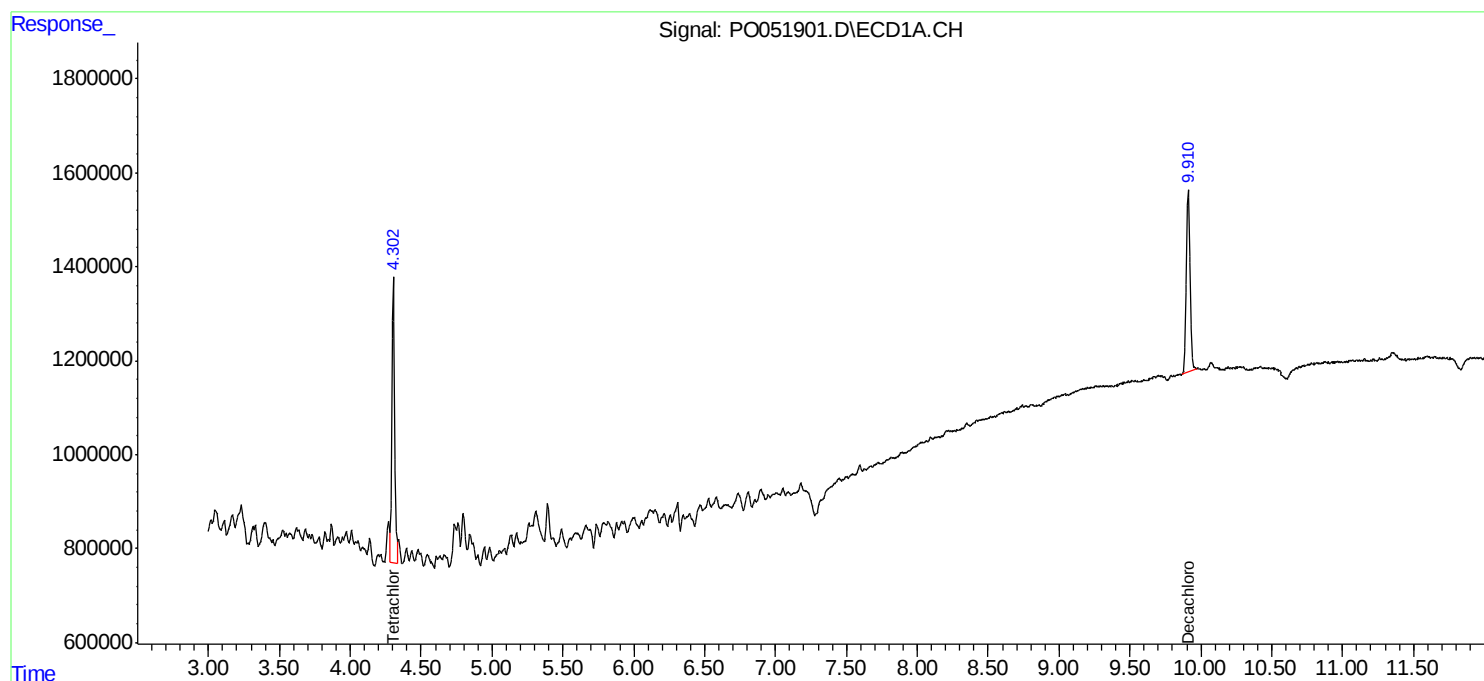

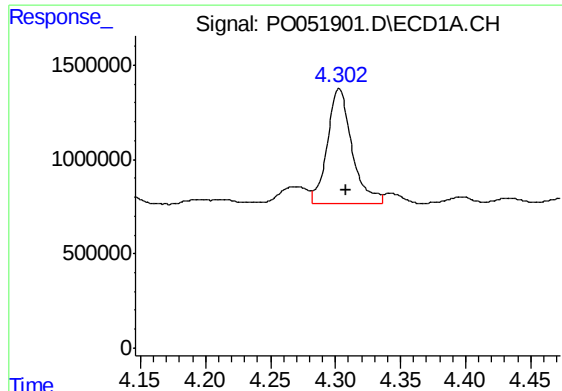


#1 Tetrachloro-m-xylene

R.T.: 4.303 min
Delta R.T.: -0.005 min
Response: 7981039
Conc: 12.23 ng/ml

Instrument :
ECD_O
ClientSampleId :
NON-UST-03R-A


Manual Integrations
APPROVED

mohammad
11/29/2018 2:24:31 PM

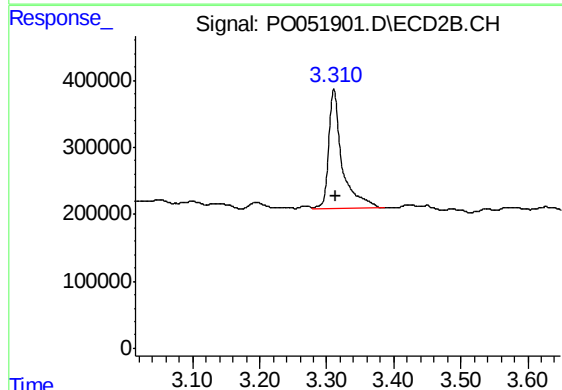


#1 Tetrachloro-m-xylene

R.T.: 3.311 min
Delta R.T.: -0.003 min
Response: 2471726
Conc: 10.47 ng/ml

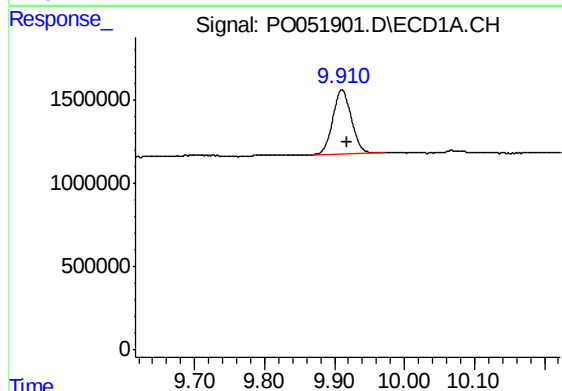

#2 Decachlorobiphenyl

R.T.: 9.910 min
Delta R.T.: -0.008 min
Response: 7148487
Conc: 17.14 ng/ml m

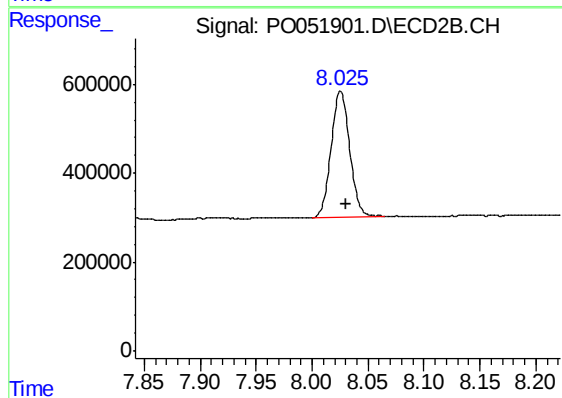

#2 Decachlorobiphenyl

R.T.: 8.025 min
Delta R.T.: -0.004 min
Response: 3278736
Conc: 16.57 ng/ml