

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112818\
 Data File : P0051919.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Nov 2018 19:38
 Operator : SM/SJ
 Sample : J6078-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 112618-JETT-F-D-B

Manual Integrations
 APPROVED

mohammad
 11/29/2018 2:24:54 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 08:12:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.299	3.307	16510392	4940041	25.309	20.923
2) SA Decachlor...	9.903	8.021	7851593	3772961	18.829	19.070m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112818\
Data File : PO051919.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Nov 2018 19:38
Operator : SM/SJ
Sample : J6078-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
112618-JETT-F-D-B


Manual Integrations
APPROVED

mohammad
11/29/2018 2:24:54 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 08:12:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

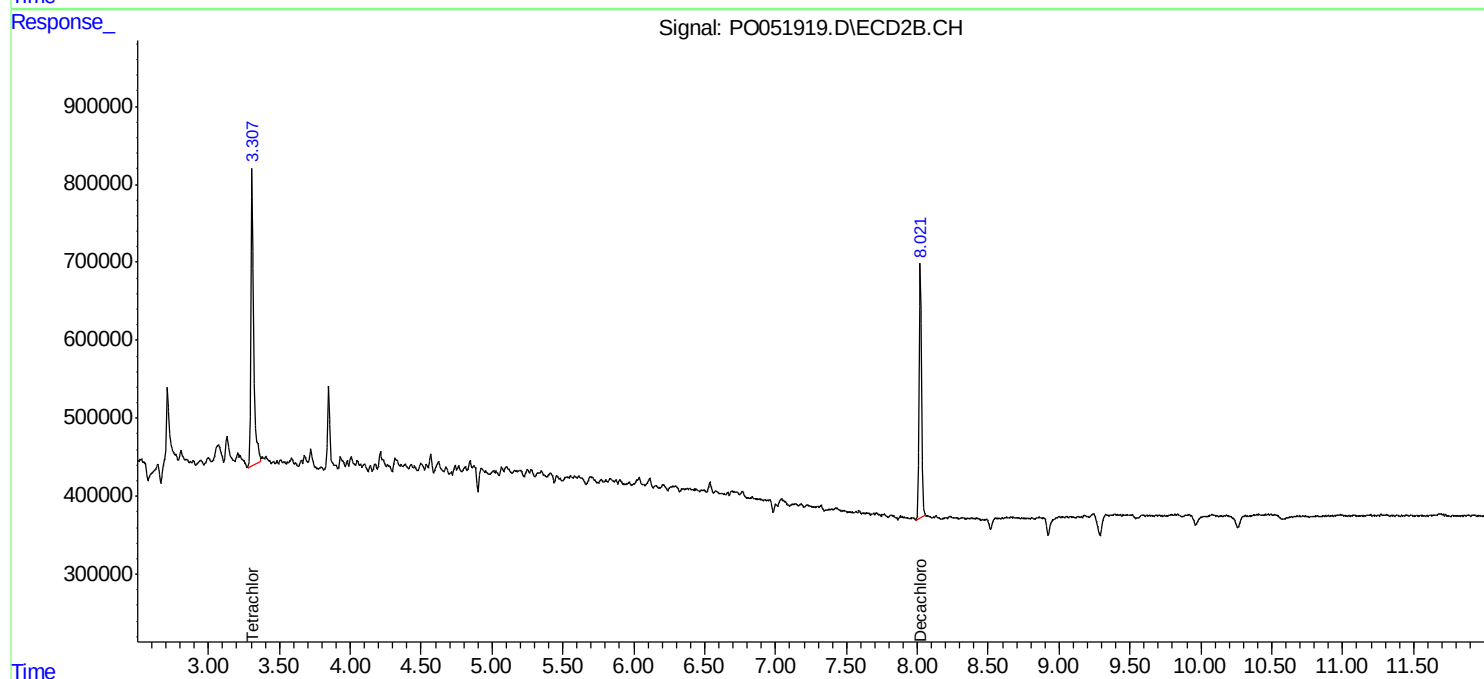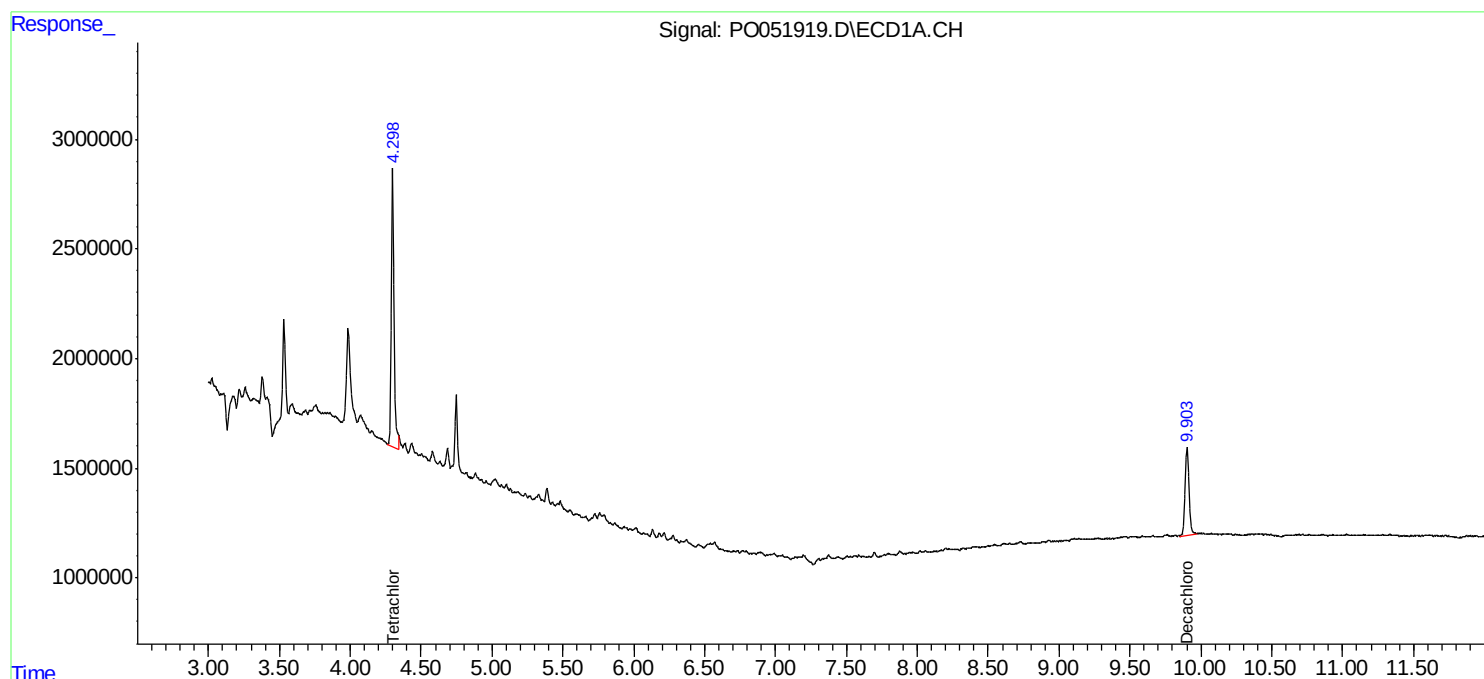

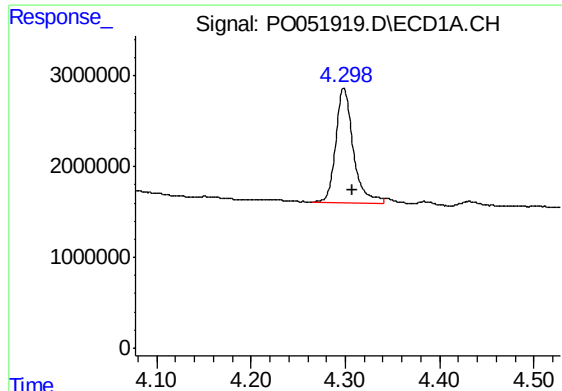


#1 Tetrachloro-m-xylene

R.T.: 4.299 min
Delta R.T.: -0.009 min
Response: 16510392
Conc: 25.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
112618-JETT-F-D-B


Manual Integrations
APPROVED

mohammad
11/29/2018 2:24:54 PM

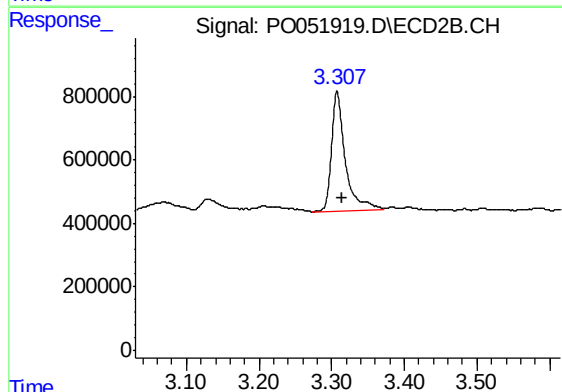


#1 Tetrachloro-m-xylene

R.T.: 3.307 min
Delta R.T.: -0.007 min
Response: 4940041
Conc: 20.92 ng/ml

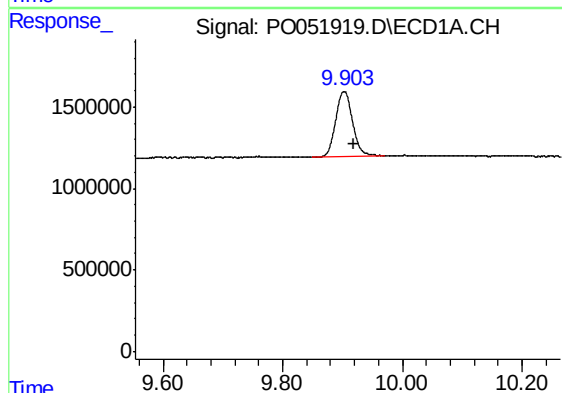

#2 Decachlorobiphenyl

R.T.: 9.903 min
Delta R.T.: -0.015 min
Response: 7851593
Conc: 18.83 ng/ml

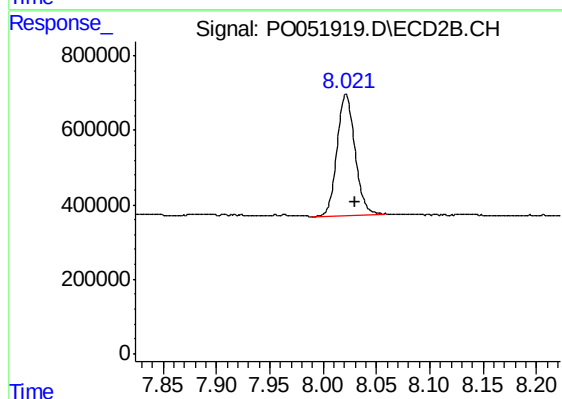

#2 Decachlorobiphenyl

R.T.: 8.021 min
Delta R.T.: -0.009 min
Response: 3772961
Conc: 19.07 ng/ml m