

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112818\
 Data File : P0051921.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Nov 2018 20:12
 Operator : SM/SJ
 Sample : J6078-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 112618-JETT-F-D-S

Manual Integrations
 APPROVED

mohammad
 11/29/2018 2:24:56 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 08:13:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.298	3.307	16000550	4397492	24.527	18.626
2) SA Decachlor...	9.904	8.021	6777022	3257148	16.252	16.463m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112818\
Data File : PO051921.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Nov 2018 20:12
Operator : SM/SJ
Sample : J6078-03
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
112618-JETT-F-D-S


Manual Integrations
APPROVED

mohammad
11/29/2018 2:24:56 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 08:13:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

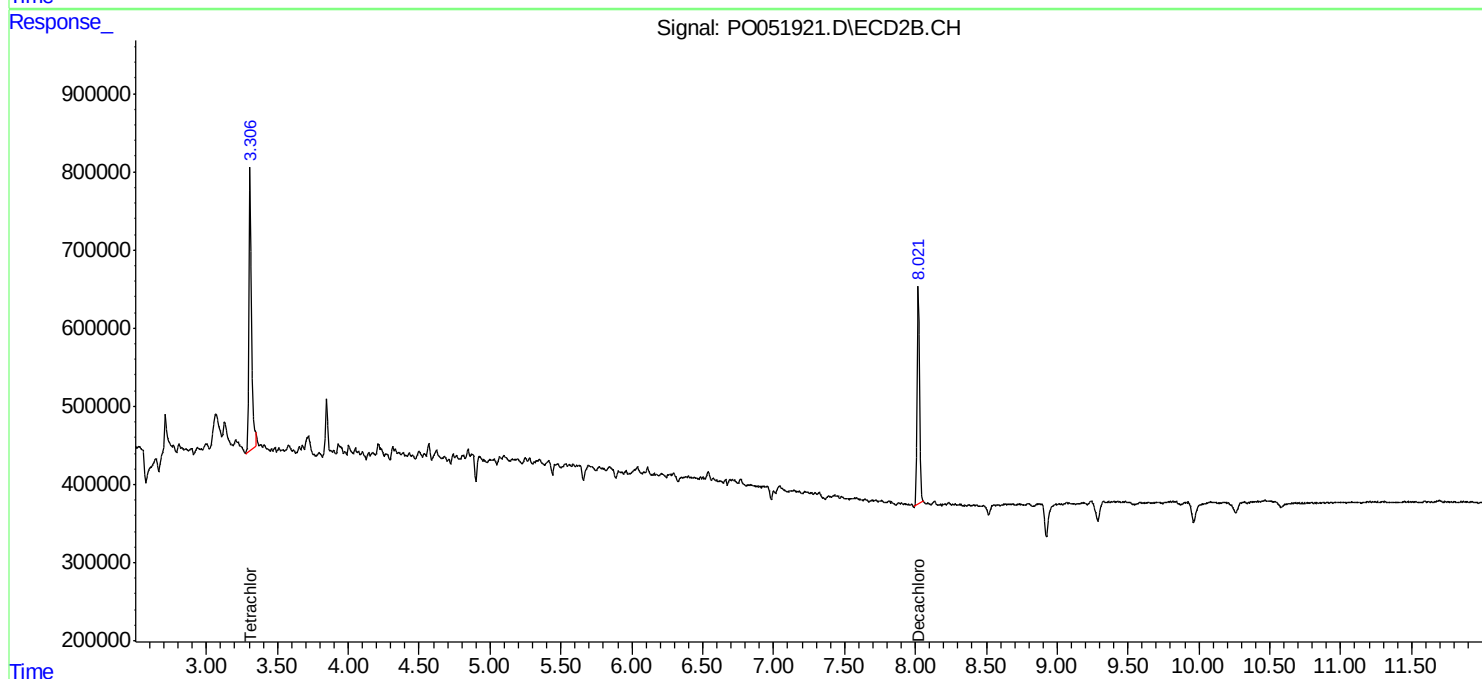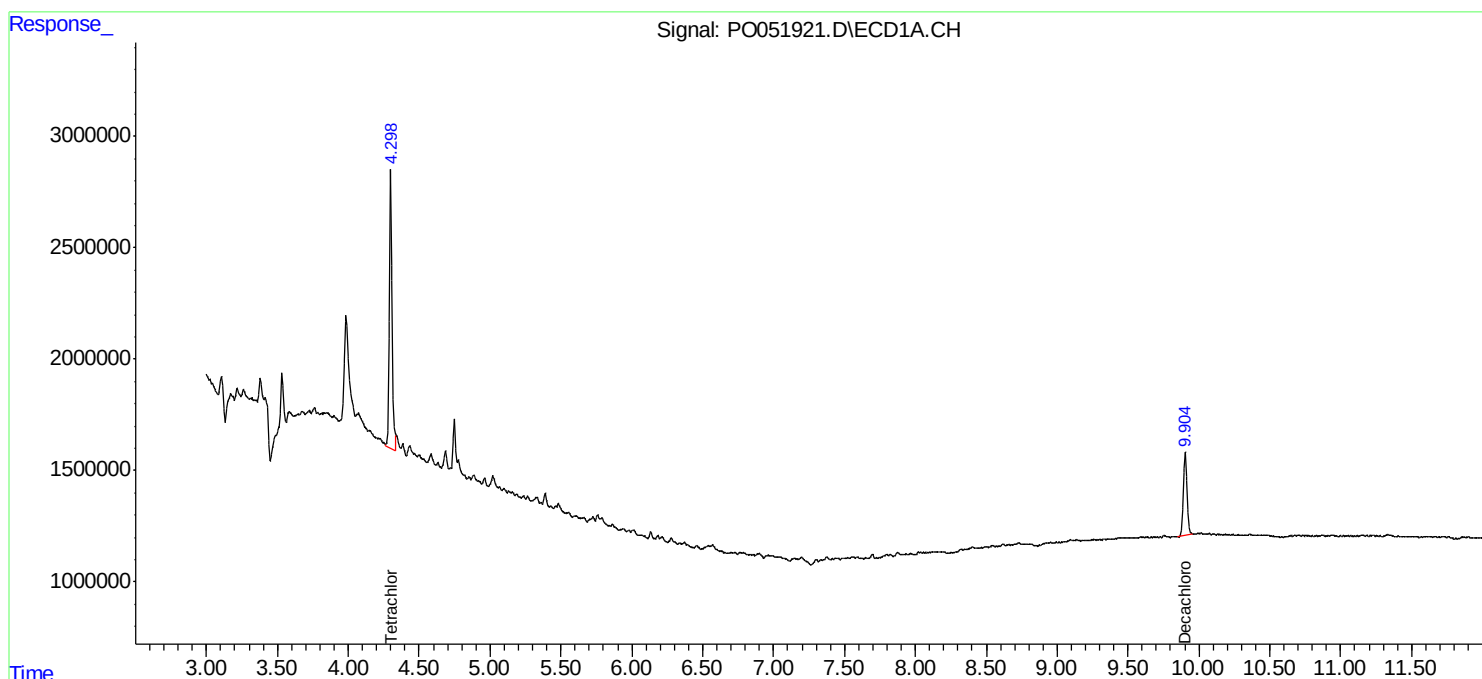

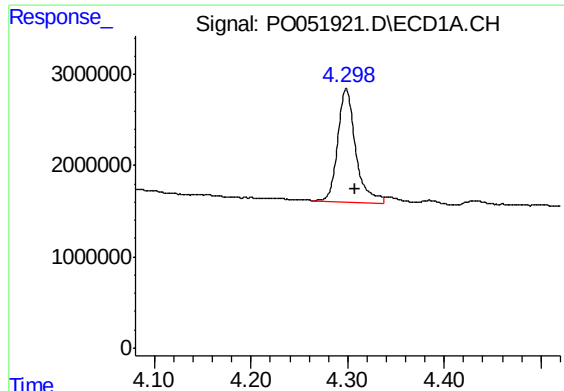


#1 Tetrachloro-m-xylene

R.T.: 4.298 min
Delta R.T.: -0.010 min
Response: 16000550
Conc: 24.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
112618-JETT-F-D-S


Manual Integrations
APPROVED

mohammad
11/29/2018 2:24:56 PM

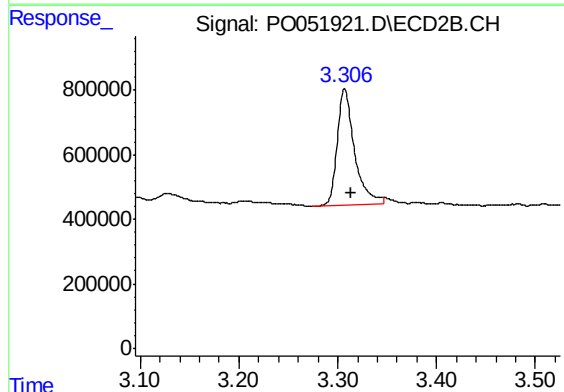


#1 Tetrachloro-m-xylene

R.T.: 3.307 min
Delta R.T.: -0.007 min
Response: 4397492
Conc: 18.63 ng/ml

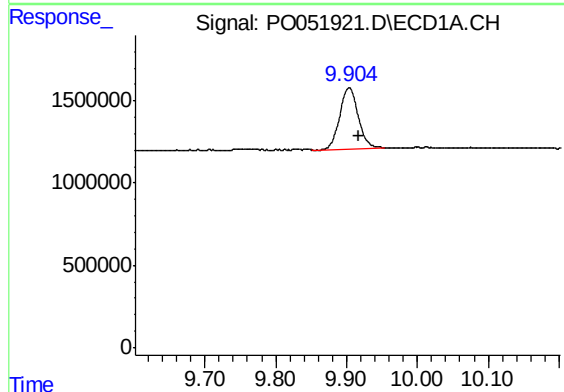

#2 Decachlorobiphenyl

R.T.: 9.904 min
Delta R.T.: -0.014 min
Response: 6777022
Conc: 16.25 ng/ml

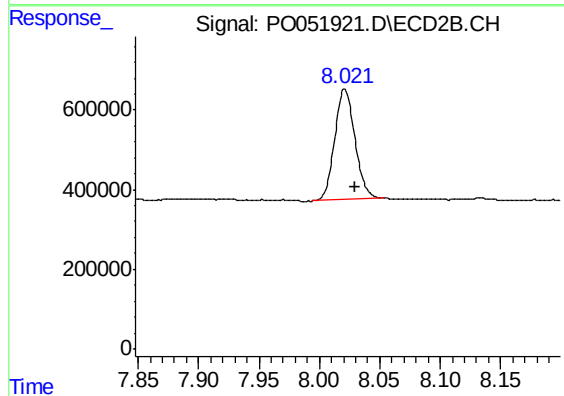

#2 Decachlorobiphenyl

R.T.: 8.021 min
Delta R.T.: -0.009 min
Response: 3257148
Conc: 16.46 ng/ml m