

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112818\
 Data File : P0051941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 29 Nov 2018 1:51
 Operator : SM/SJ
 Sample : J6013-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DISPOSAL-WASTE-CLASS

Manual Integrations
 APPROVED

mohammad
 11/29/2018 2:26:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 29 08:24:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 27 01:06:37 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.297	3.306	15836014	4690960	24.275	19.869
2) SA Decachlor...	9.901	8.020	9163445	4486508	21.975	22.677m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112818\
Data File : PO051941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Nov 2018 1:51
Operator : SM/SJ
Sample : J6013-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DISPOSAL-WASTE-CLASS


Manual Integrations
APPROVED

mohammad
11/29/2018 2:26:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 08:24:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

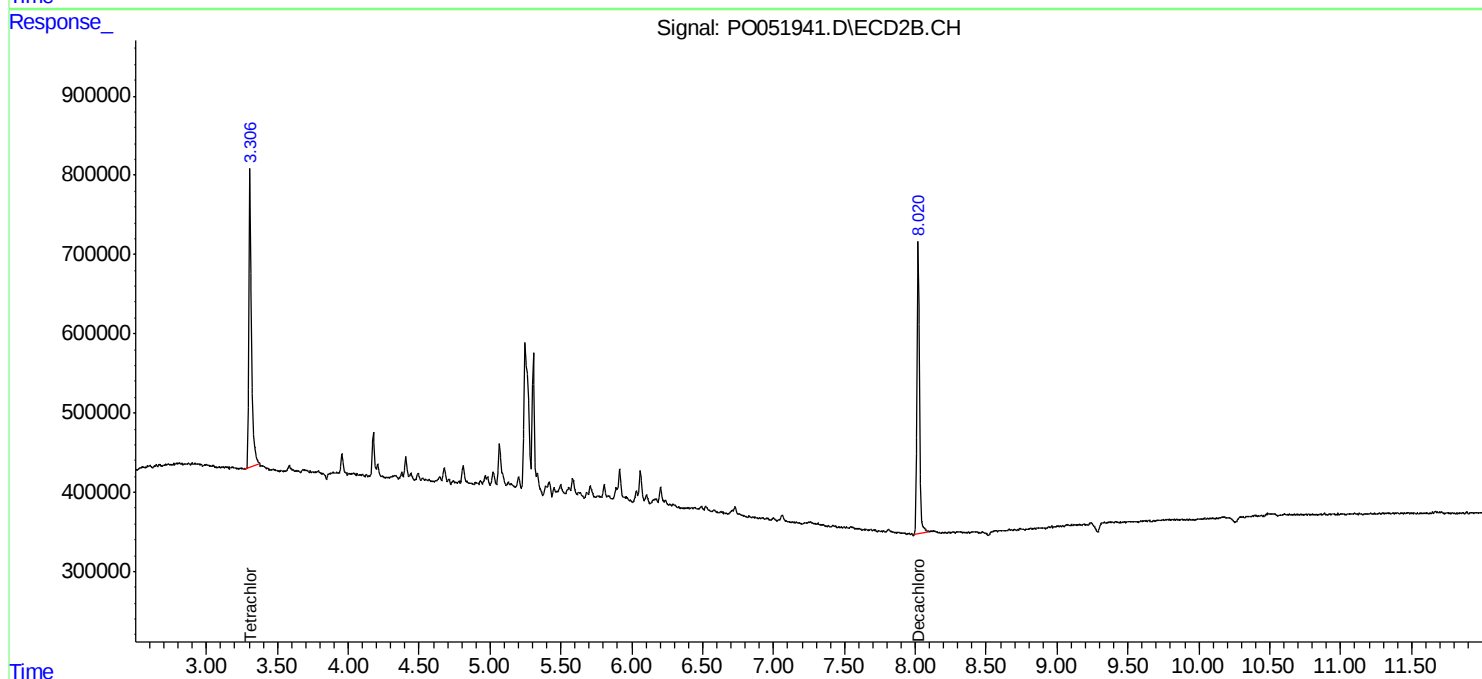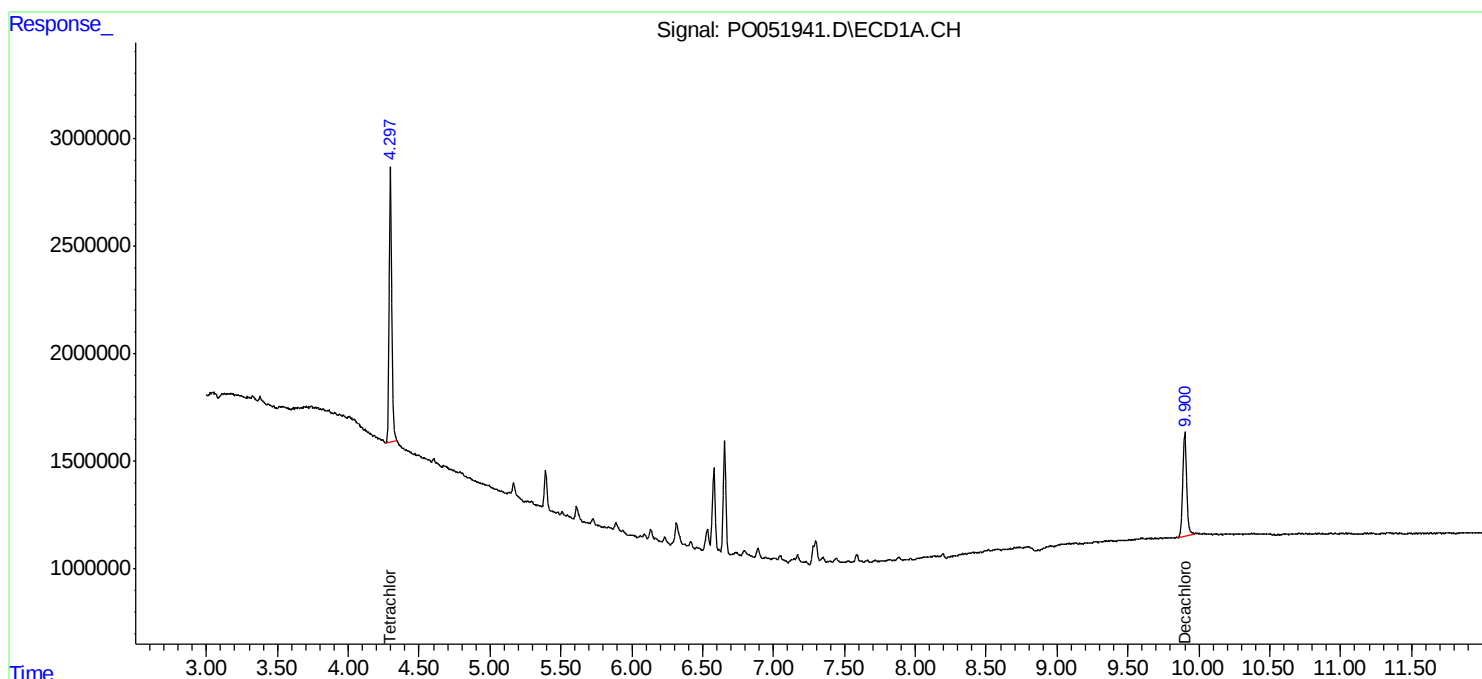

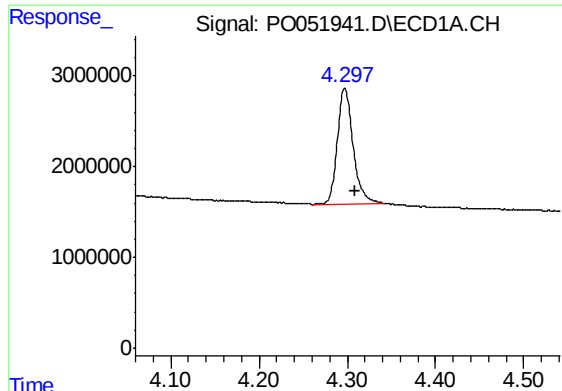


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.011 min
Response: 15836014
Conc: 24.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
DISPOSAL-WASTE-CLASS


Manual Integrations
APPROVED

mohammad
11/29/2018 2:26:01 PM

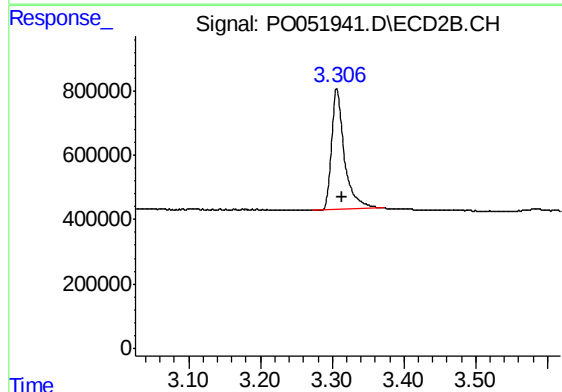


#1 Tetrachloro-m-xylene

R.T.: 3.306 min
Delta R.T.: -0.008 min
Response: 4690960
Conc: 19.87 ng/ml

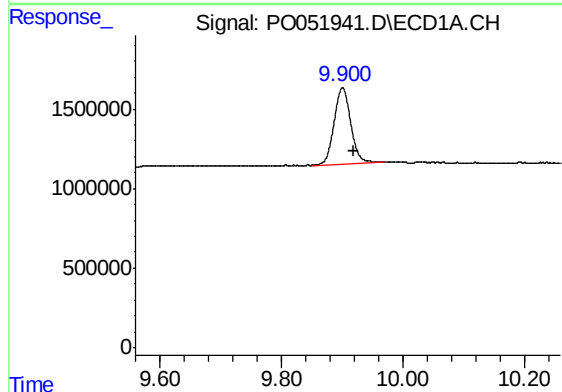

#2 Decachlorobiphenyl

R.T.: 9.901 min
Delta R.T.: -0.017 min
Response: 9163445
Conc: 21.98 ng/ml

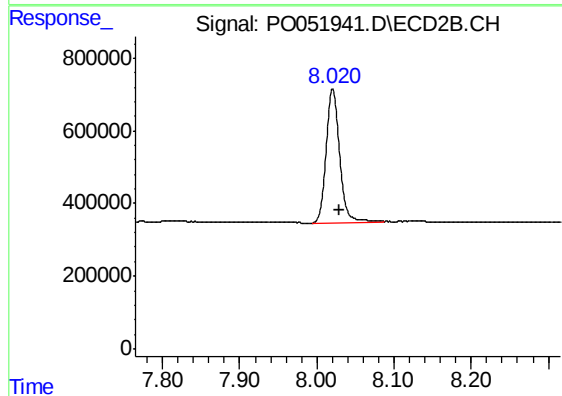

#2 Decachlorobiphenyl

R.T.: 8.020 min
Delta R.T.: -0.010 min
Response: 4486508
Conc: 22.68 ng/ml m