

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0112818\
Data File : P0051948.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Nov 2018 3:49
Operator : SM/SJ
Sample : J6060-08
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
20180948-SITE-WATER

Manual Integrations
APPROVED

mohammad
11/29/2018 2:26:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 08:30:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.297	3.308	13380690	4143340	20.511	17.549
2) SA Decachlor...	9.898	8.019	10204619	4731789	24.472	23.917m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO112818\
Data File : PO051948.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 29 Nov 2018 3:49
Operator : SM/SJ
Sample : J6060-08
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
20180948-SITE-WATER


Manual Integrations
APPROVED

mohammad
11/29/2018 2:26:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 29 08:30:17 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112618.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 27 01:06:37 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

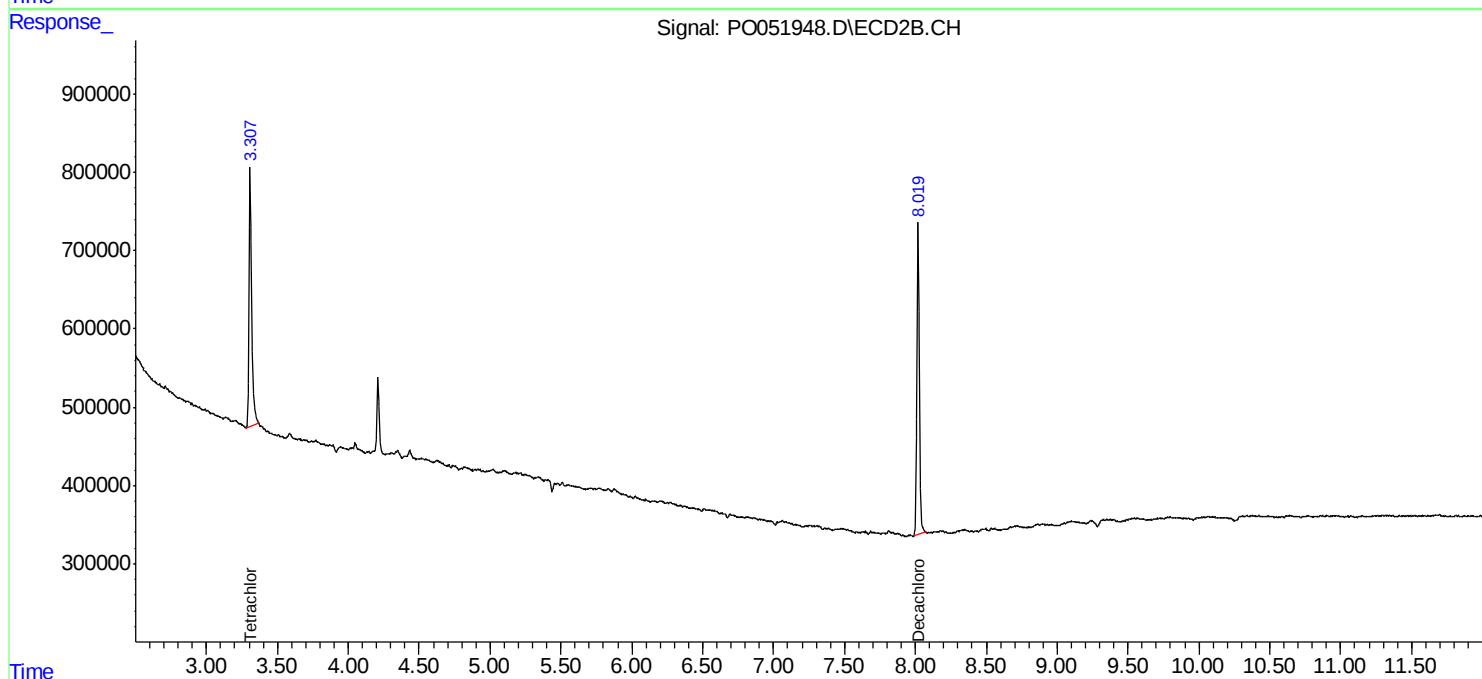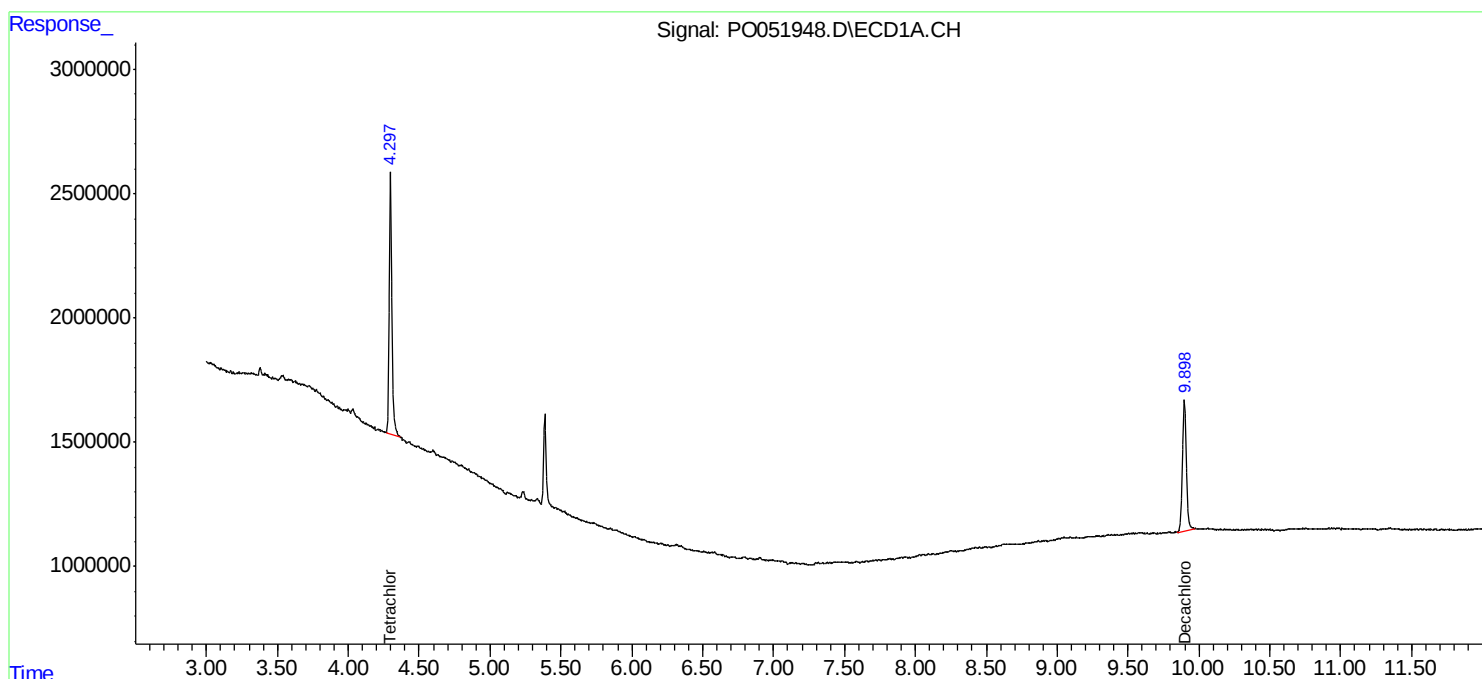

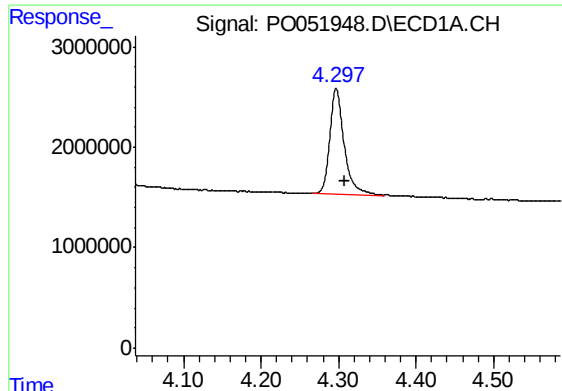


#1 Tetrachloro-m-xylene

R.T.: 4.297 min
Delta R.T.: -0.011 min
Response: 13380690
Conc: 20.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
20180948-SITE-WATER


Manual Integrations
APPROVED

mohammad
11/29/2018 2:26:22 PM

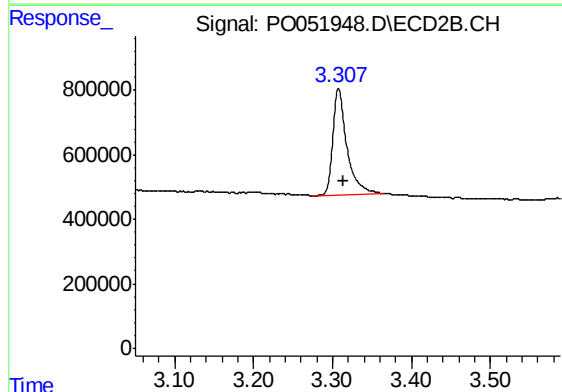


#1 Tetrachloro-m-xylene

R.T.: 3.308 min
Delta R.T.: -0.006 min
Response: 4143340
Conc: 17.55 ng/ml

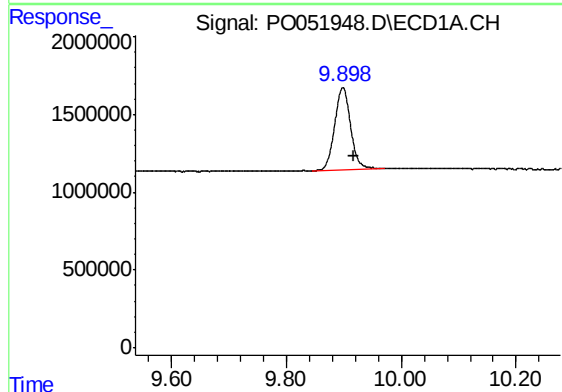

#2 Decachlorobiphenyl

R.T.: 9.898 min
Delta R.T.: -0.019 min
Response: 10204619
Conc: 24.47 ng/ml

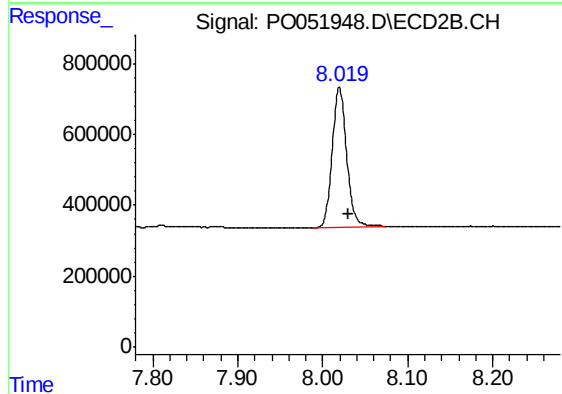

#2 Decachlorobiphenyl

R.T.: 8.019 min
Delta R.T.: -0.011 min
Response: 4731789
Conc: 23.92 ng/ml m