

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120118\
 Data File : P0052123.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2018 17:38
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 06:50:38 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 03 06:36:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.291	25695785	8932791	22.459	20.565
2) SA Decachlor...	9.867	7.999	17827603	7948024	18.777	19.946
Target Compounds						
9) L2 AR-1221-2	0.000	3.569	0	193304	N.D.	60.527 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120118\
Data File : PO052123.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2018 17:38
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 06:50:38 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 03 06:36:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

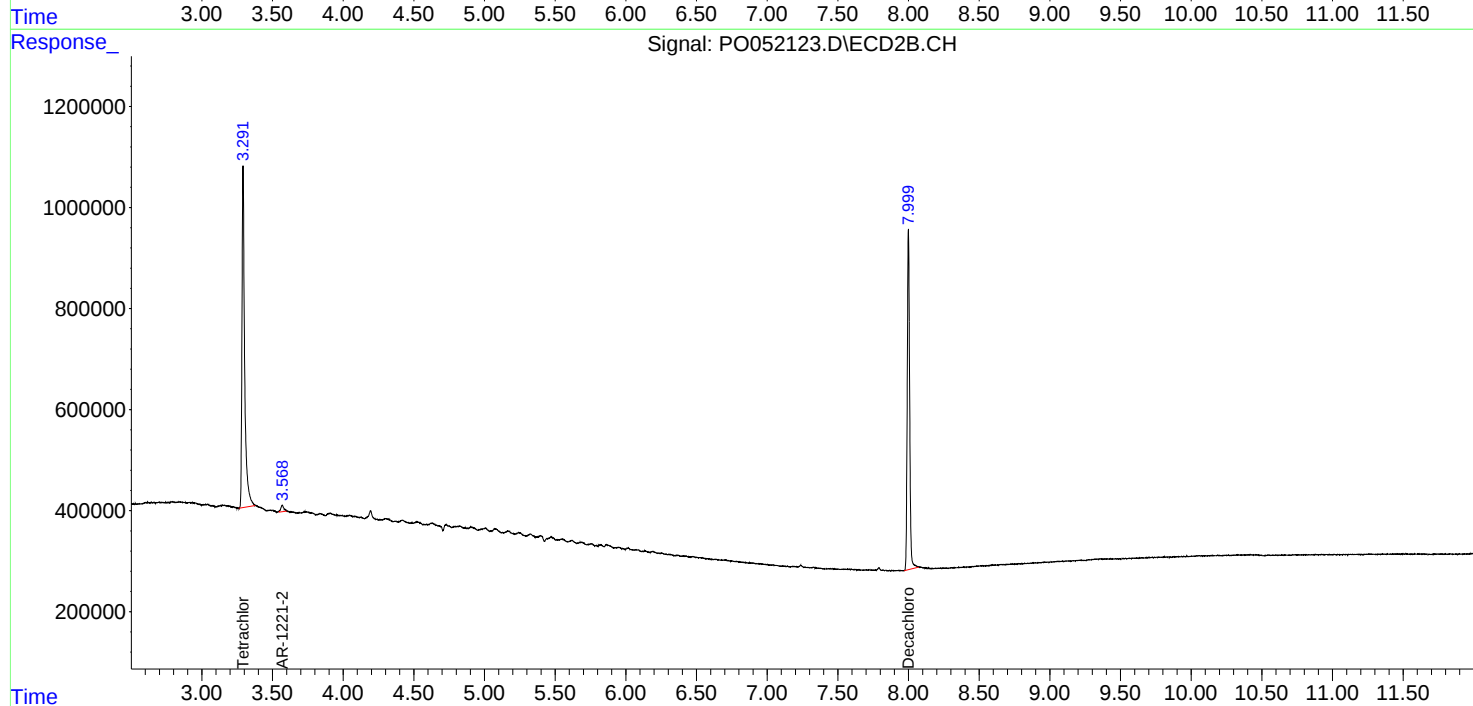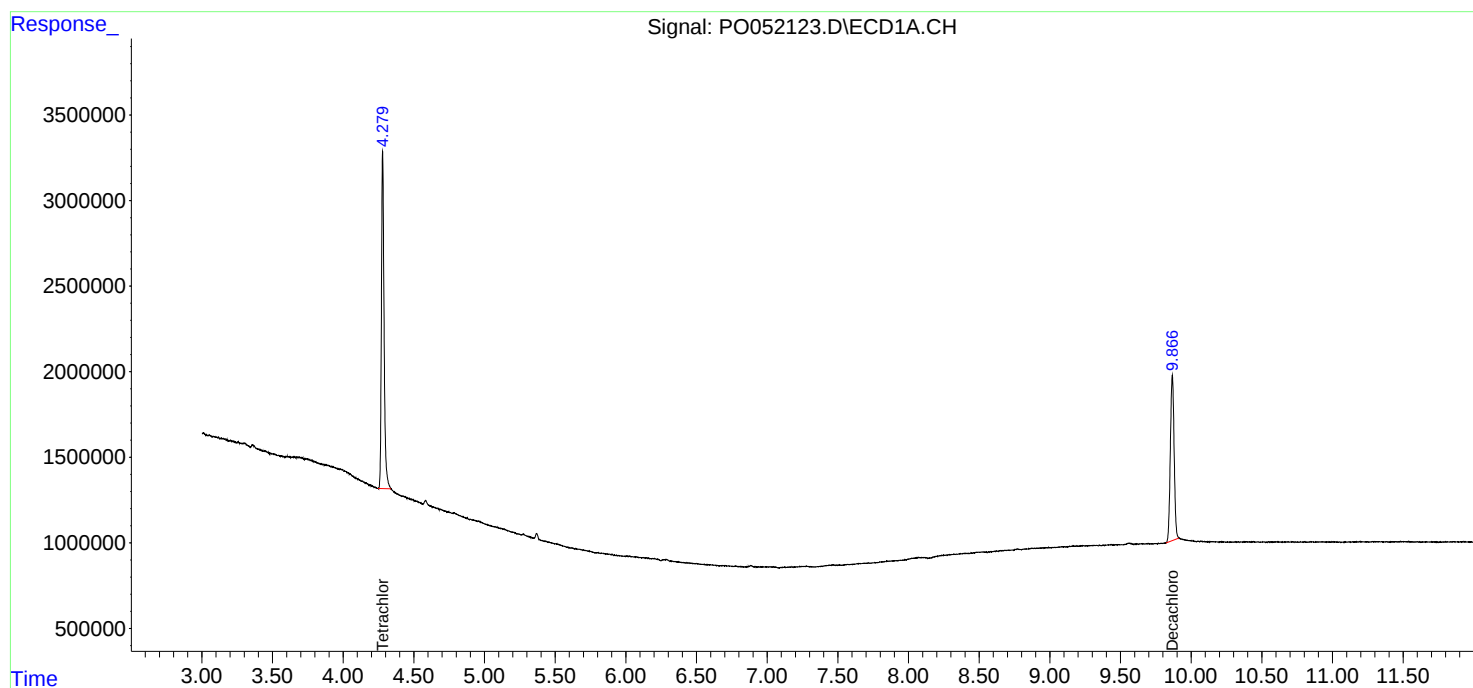


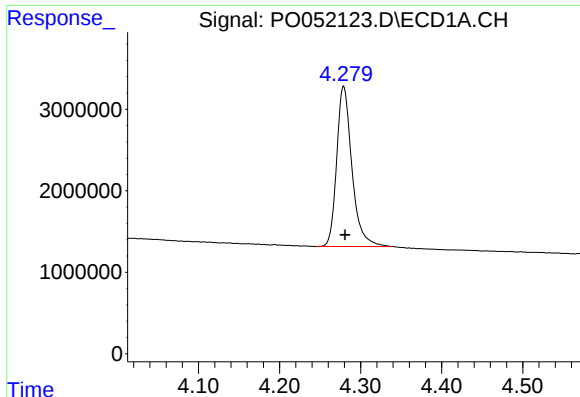

#1 Tetrachloro-m-xylene


R.T.: 4.279 min
Delta R.T.: -0.002 min
Response: 25695785
Conc: 22.46 ng/ml

Instrument :
ECD_O
ClientSampleId :

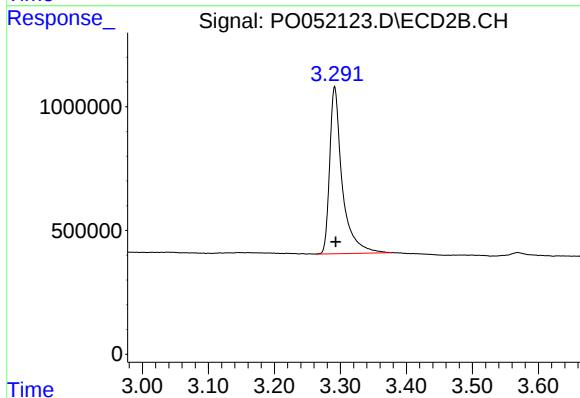


#1 Tetrachloro-m-xylene

R.T.: 3.291 min
Delta R.T.: -0.002 min
Response: 8932791
Conc: 20.56 ng/ml

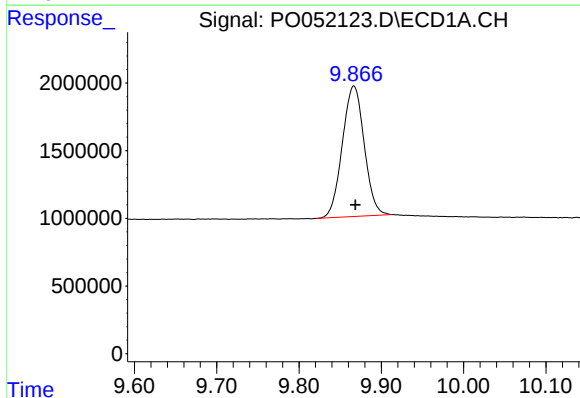


#2 Decachlorobiphenyl

R.T.: 9.867 min
Delta R.T.: -0.002 min
Response: 17827603
Conc: 18.78 ng/ml

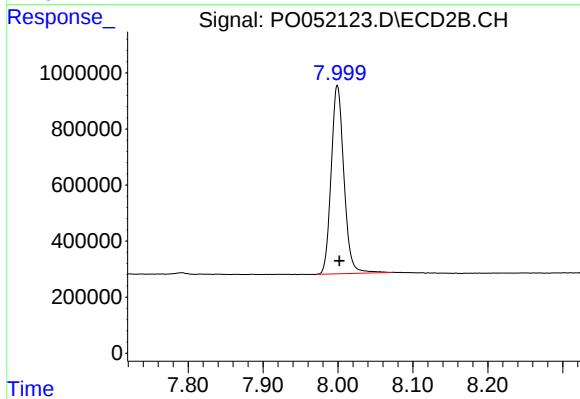

#2 Decachlorobiphenyl


R.T.: 7.999 min
Delta R.T.: -0.003 min
Response: 7948024
Conc: 19.95 ng/ml

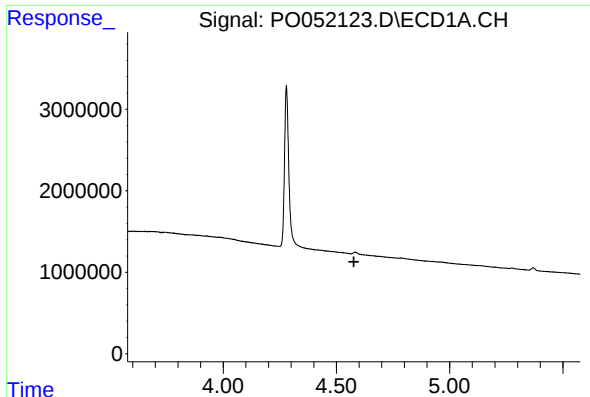

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 4.577 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

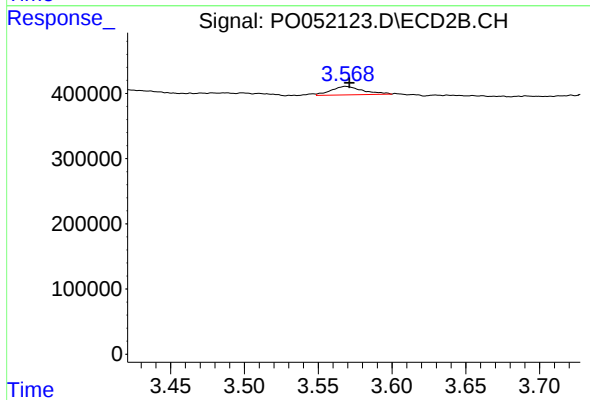

#9 AR-1221-2

R.T.: 3.569 min
Delta R.T.: -0.003 min
Response: 193304
Conc: 60.53 ng/ml