

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120118\
 Data File : P0052113.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2018 14:49
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 06:45:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 03 06:36:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.280	3.291	23734000	8448012	20.745	19.449
2)	SA Decachlor...	9.866	8.000	17779948	7949407	18.727	19.949

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120118\
Data File : P0052113.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2018 14:49
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 06:45:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 03 06:36:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

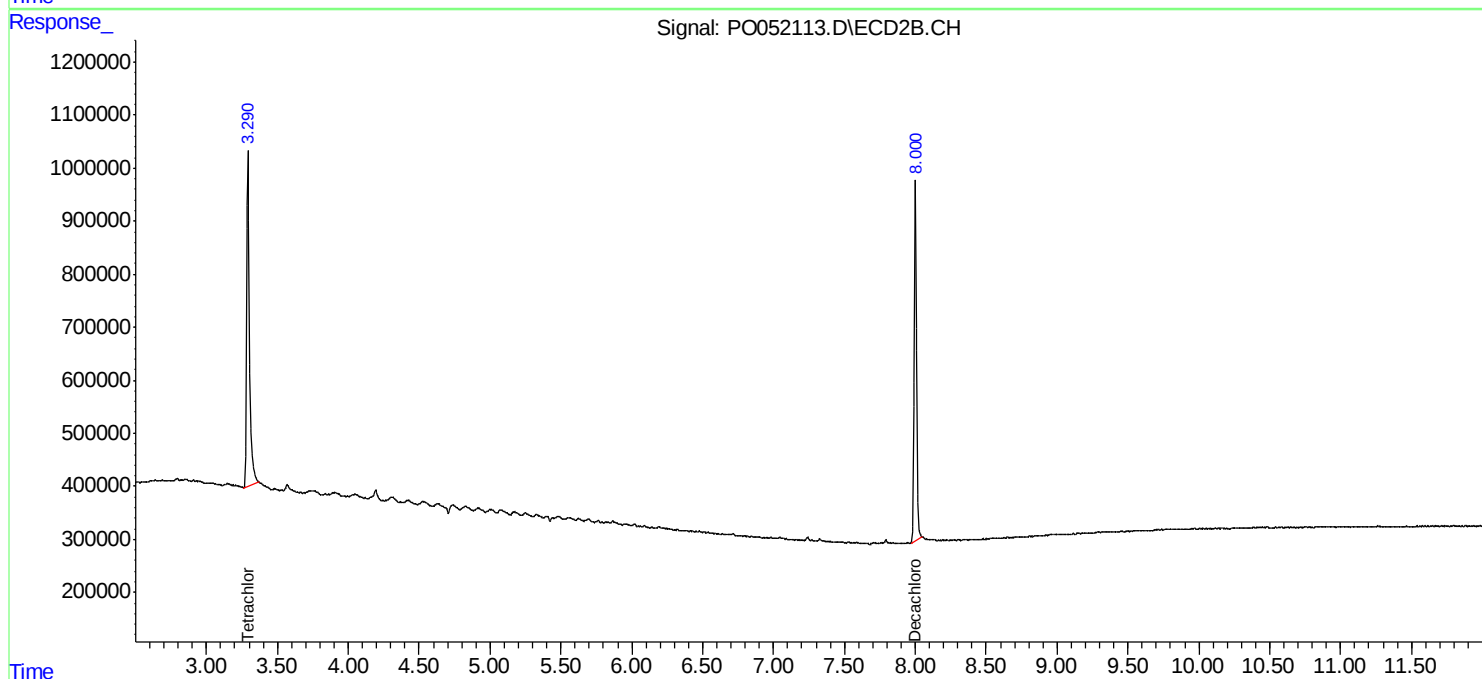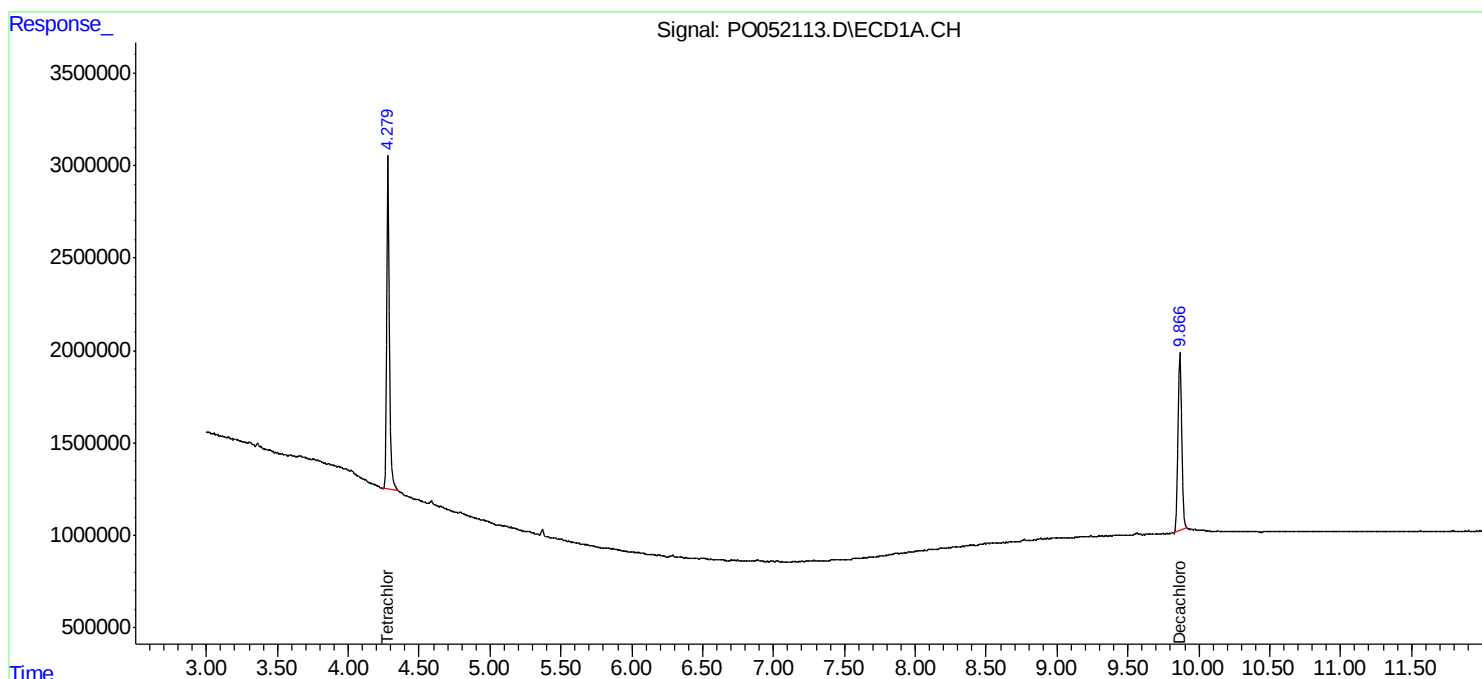


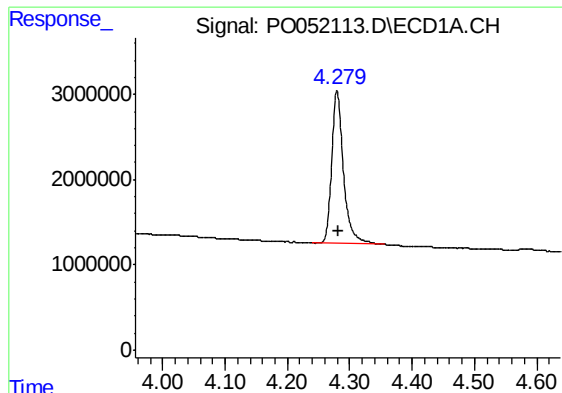

#1 Tetrachloro-m-xylene


R.T.: 4.280 min
Delta R.T.: -0.001 min
Response: 23734000
Conc: 20.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

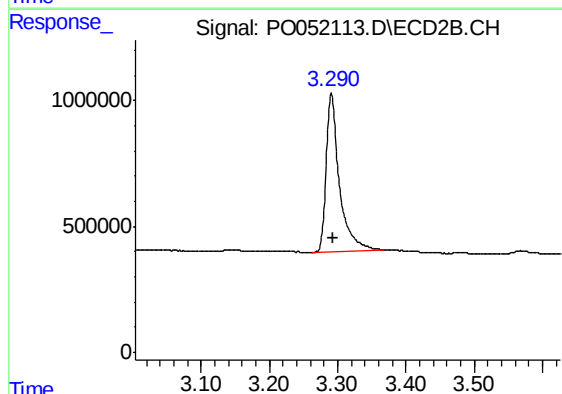


#1 Tetrachloro-m-xylene

R.T.: 3.291 min
Delta R.T.: -0.002 min
Response: 8448012
Conc: 19.45 ng/ml

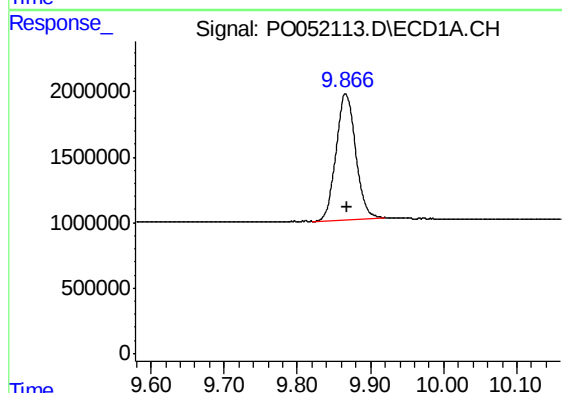

#2 Decachlorobiphenyl

R.T.: 9.866 min
Delta R.T.: -0.002 min
Response: 17779948
Conc: 18.73 ng/ml

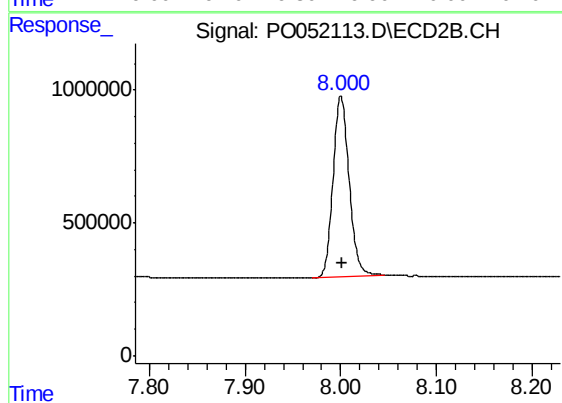

#2 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: -0.002 min
Response: 7949407
Conc: 19.95 ng/ml