

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120118\
 Data File : P0052115.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2018 15:23
 Operator : SM/SJ
 Sample : J5767-17RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CL-02-112818-ARE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 06:46:24 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 03 06:36:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.279	3.290	16364714	5250151	14.304	12.087
2) SA Decachlor...	9.866	8.000	9388238	4102555	9.888	10.295

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120118\
Data File : PO052115.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2018 15:23
Operator : SM/SJ
Sample : J5767-17RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CL-02-112818-ARE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 06:46:24 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 03 06:36:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

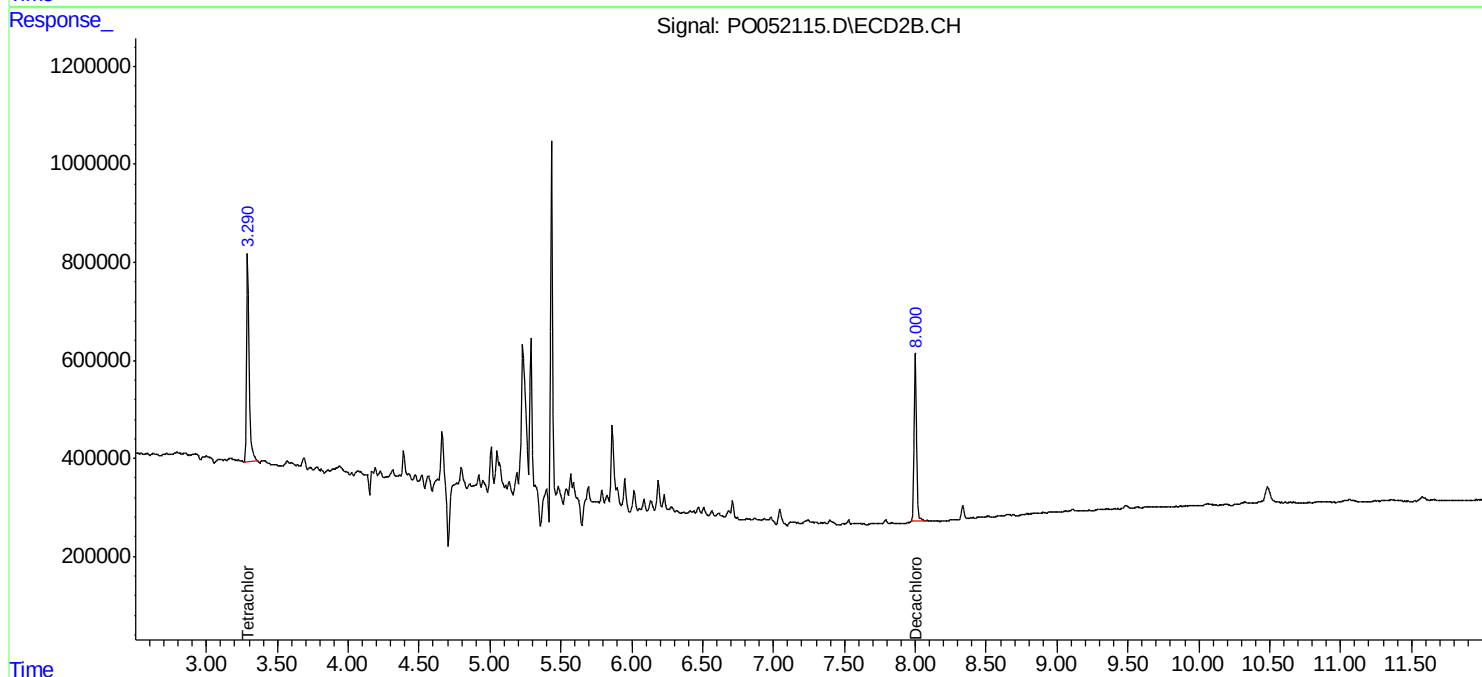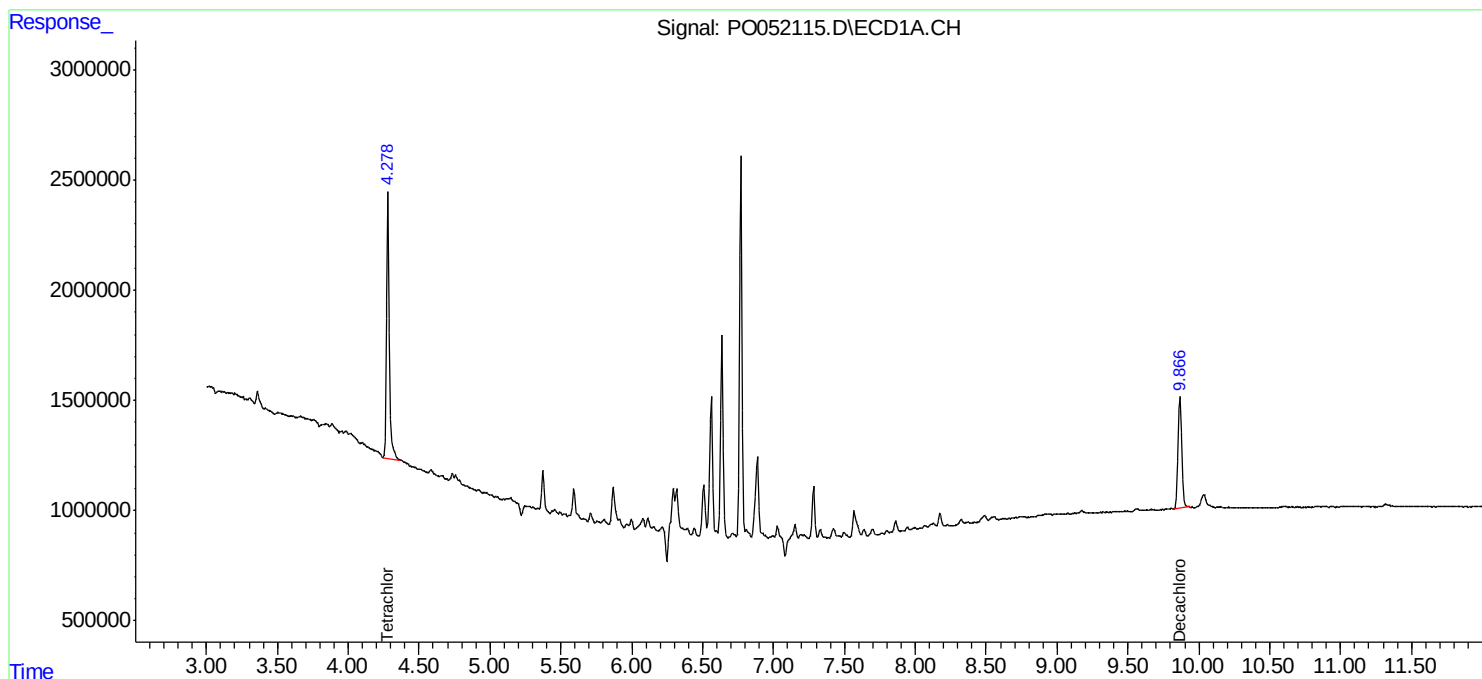


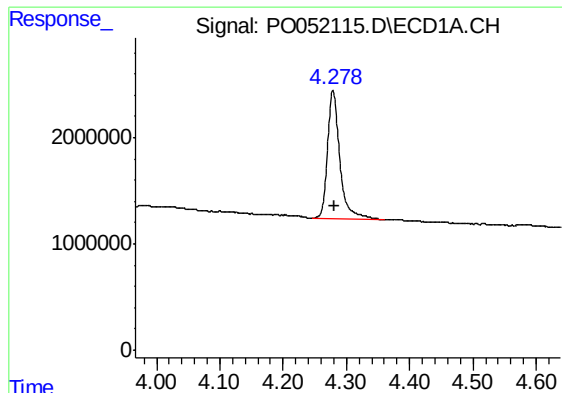

#1 Tetrachloro-m-xylene


R.T.: 4.279 min
Delta R.T.: -0.002 min
Response: 16364714
Conc: 14.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
CL-02-112818-ARE

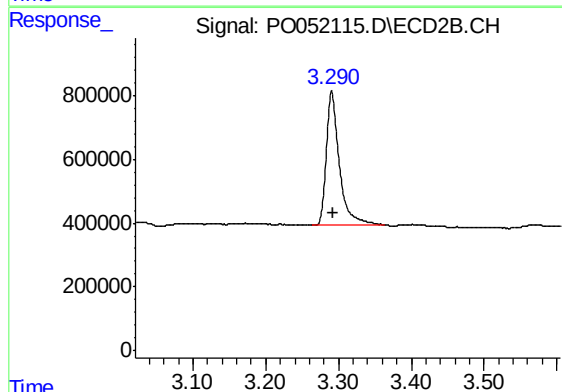


#1 Tetrachloro-m-xylene

R.T.: 3.290 min
Delta R.T.: -0.002 min
Response: 5250151
Conc: 12.09 ng/ml

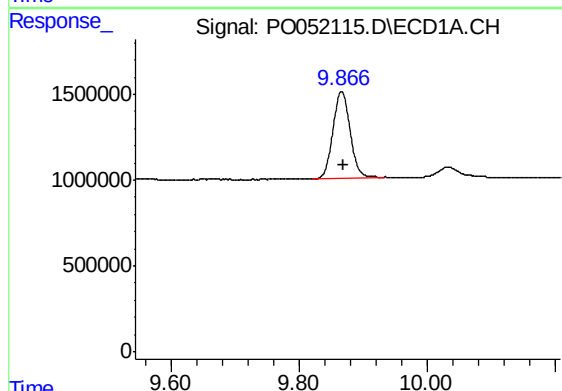

#2 Decachlorobiphenyl

R.T.: 9.866 min
Delta R.T.: -0.002 min
Response: 9388238
Conc: 9.89 ng/ml

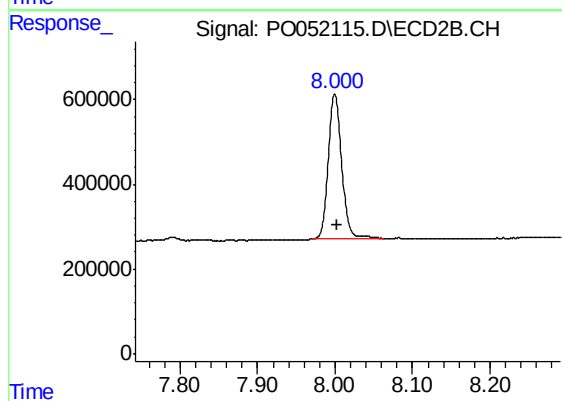

#2 Decachlorobiphenyl

R.T.: 8.000 min
Delta R.T.: -0.002 min
Response: 4102555
Conc: 10.30 ng/ml