

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120118\
 Data File : P0052118.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Dec 2018 16:14
 Operator : SM/SJ
 Sample : J5768-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 OK-01-112818

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 03 06:48:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120118.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Dec 03 06:36:10 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.279	3.292	18232246	6980425	15.936	16.070
2)	SA Decachlor...	9.866	8.001	11921542	4653204	12.557	11.677

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120118\
Data File : PO052118.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Dec 2018 16:14
Operator : SM/SJ
Sample : J5768-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
OK-01-112818

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 03 06:48:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120118.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Dec 03 06:36:10 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

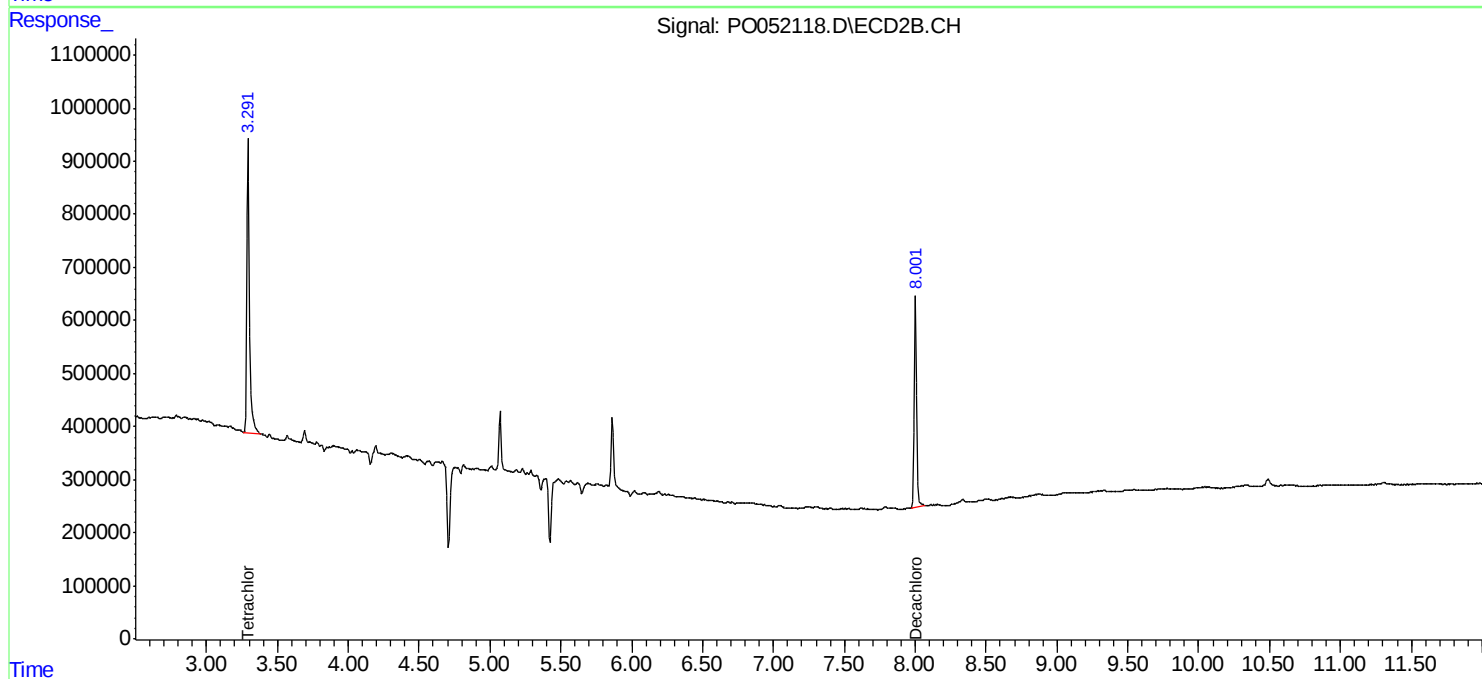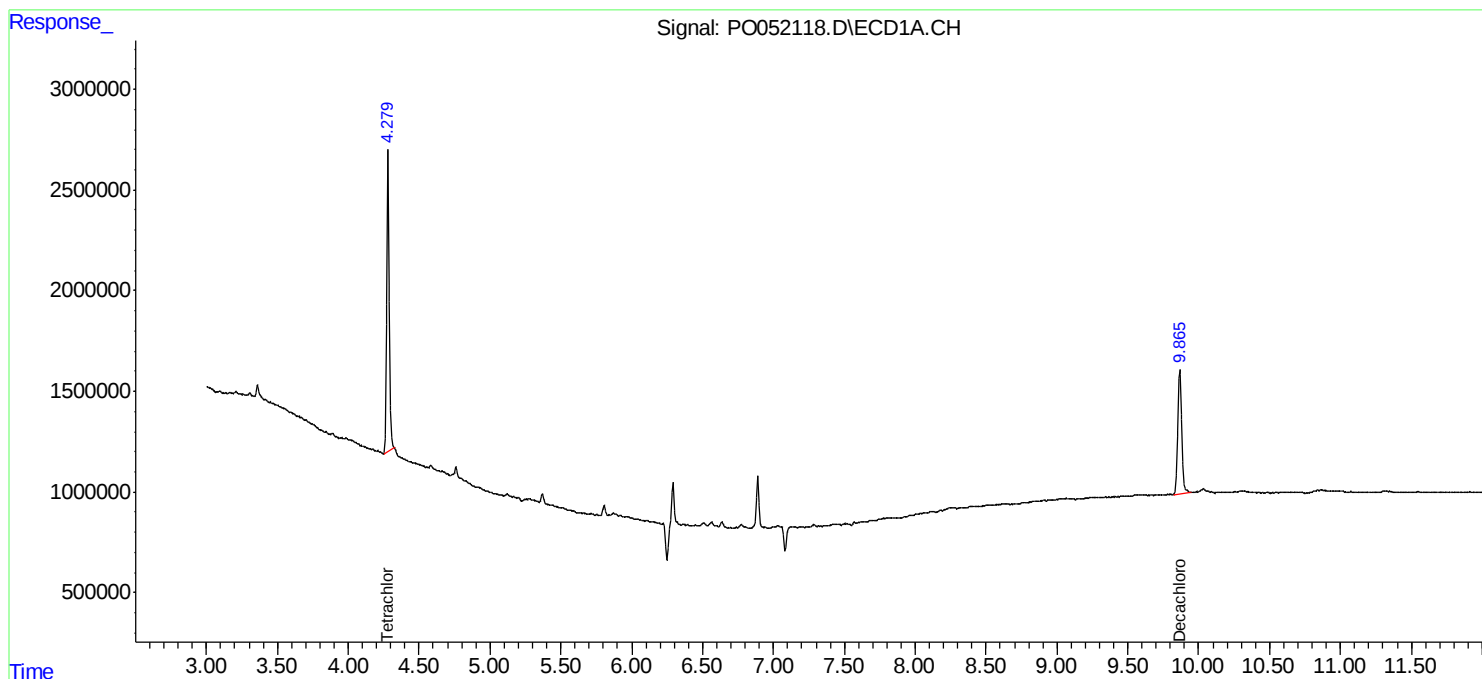


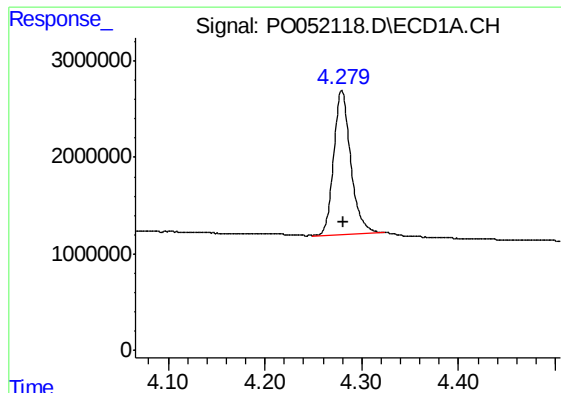

#1 Tetrachloro-m-xylene


R.T.: 4.279 min
Delta R.T.: -0.002 min
Response: 18232246
Conc: 15.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
OK-01-112818

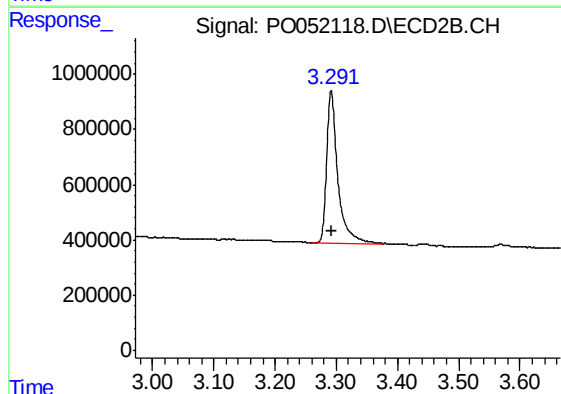


#1 Tetrachloro-m-xylene

R.T.: 3.292 min
Delta R.T.: -0.001 min
Response: 6980425
Conc: 16.07 ng/ml

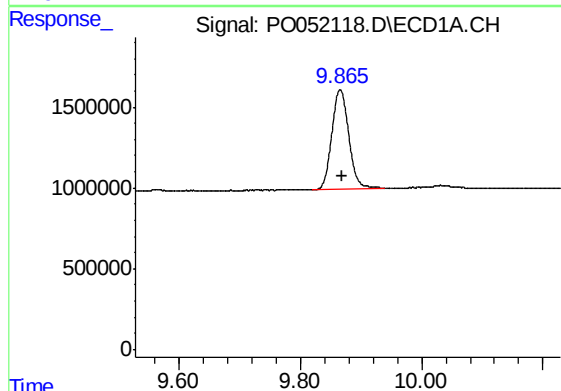

#2 Decachlorobiphenyl

R.T.: 9.866 min
Delta R.T.: -0.002 min
Response: 11921542
Conc: 12.56 ng/ml

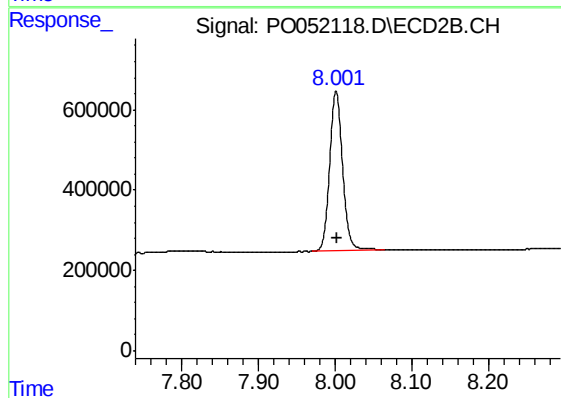

#2 Decachlorobiphenyl

R.T.: 8.001 min
Delta R.T.: 0.000 min
Response: 4653204
Conc: 11.68 ng/ml