

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
 Data File : PL042744.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Dec 2018 04:48
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 05:49:34 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
 Quant Title : GC Extractables
 QLast Update : Tue Nov 20 02:29:59 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.467	4.102	116.5E6	61239971	19.799	21.292
28)	SA Decachlor...	8.205	9.235	124.3E6	51372426	19.725	21.300
Target Compounds							
6)	B beta-BHC	4.402f	4.905f	3848861	1704411	1.086	1.080
8)	B Heptachlo...	0.000	5.996	0	3716490	N.D.	1.037 #
13)	MA Dieldrin	5.706f	0.000	200364	0	0.027	N.D. #
14)	MA Endrin	6.022	0.000	1358991	0	0.208	N.D. #
23)	Chlordane-1	4.402	0.000	3848861	0	13.921	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL120318\
Data File : PL042744.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Dec 2018 04:48
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 05:49:34 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL112018.M
Quant Title : GC Extractables
QLast Update : Tue Nov 20 02:29:59 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

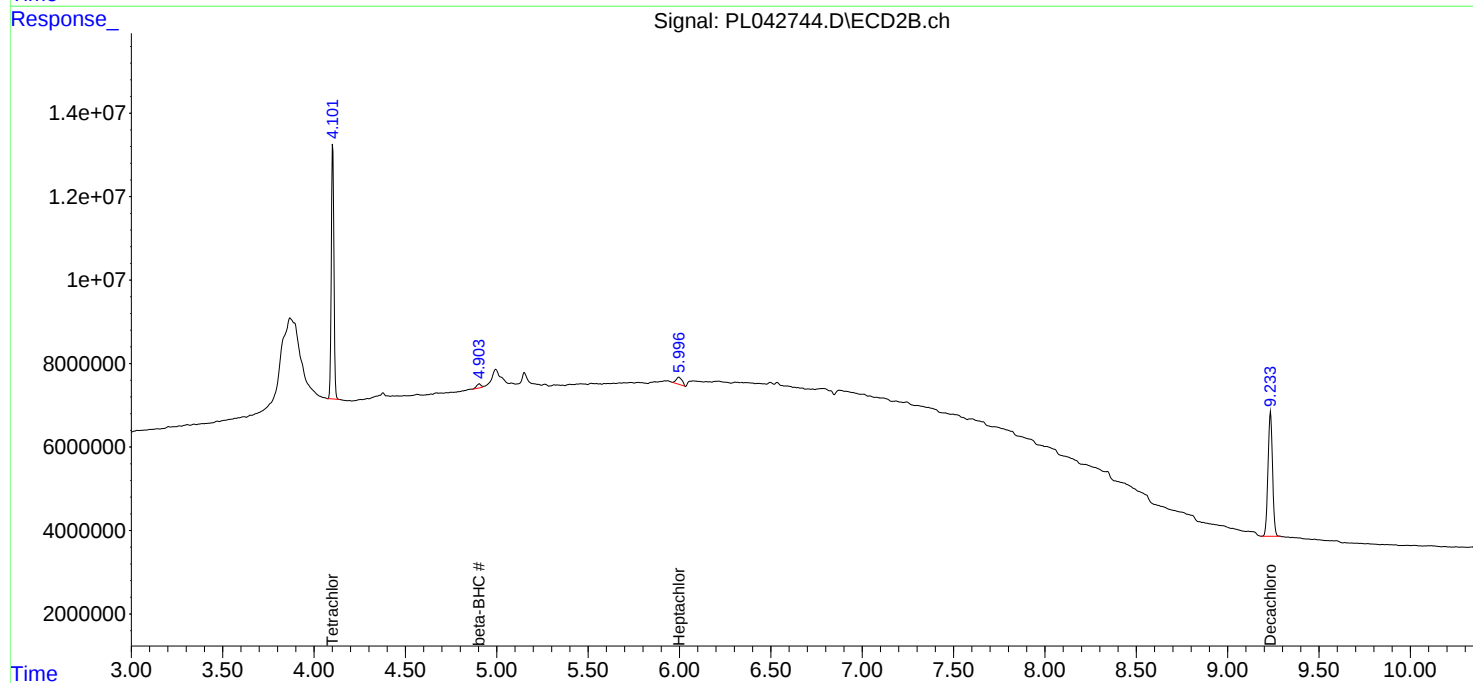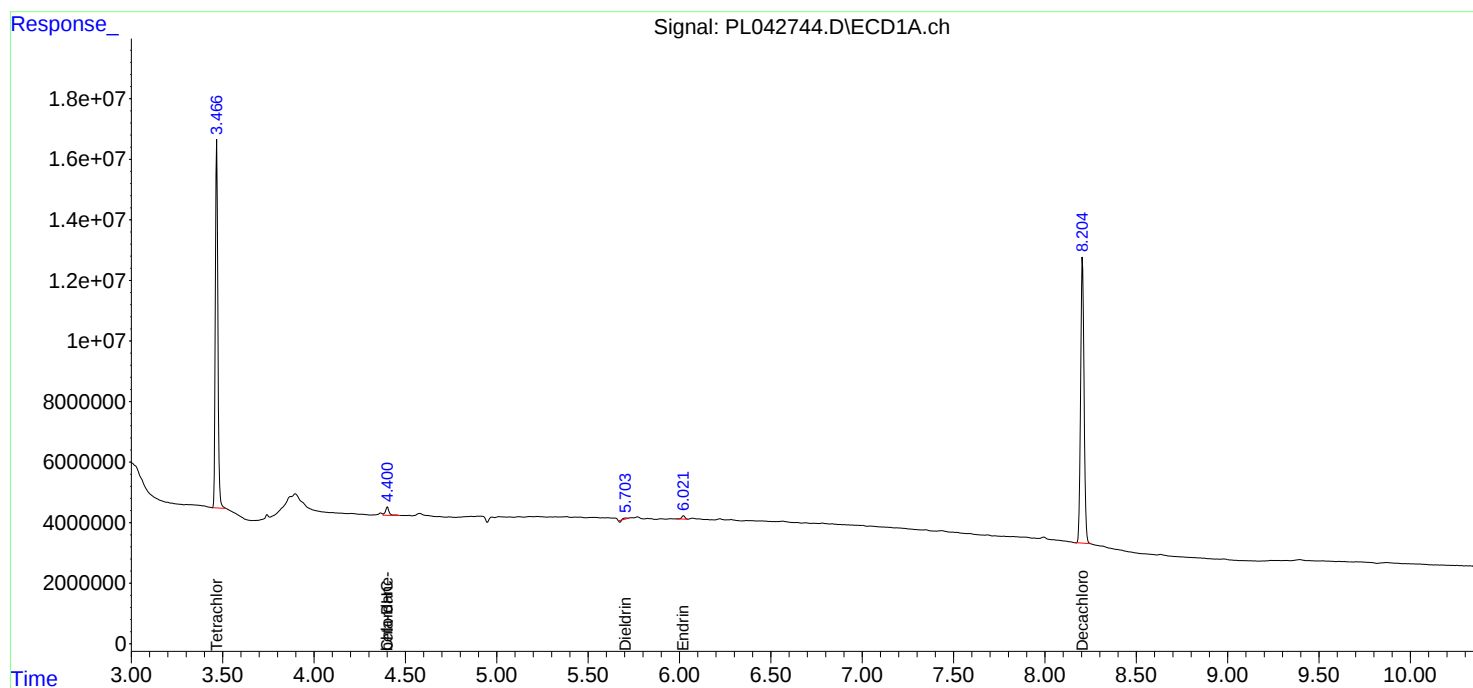


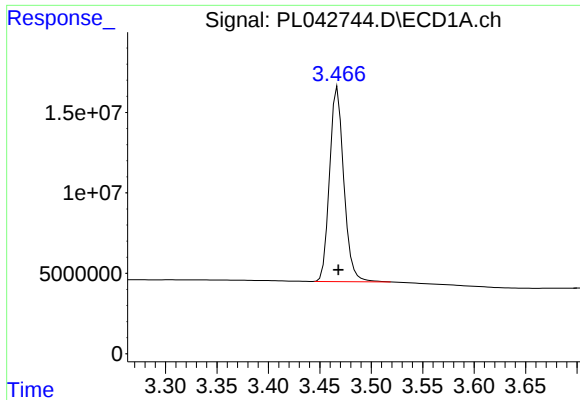

#1 Tetrachloro-m-xylene


R.T.: 3.467 min
Delta R.T.: 0.000 min
Response: 116487355
Conc: 19.80 ng/ml

Instrument :
ECD_O
ClientSampleId :

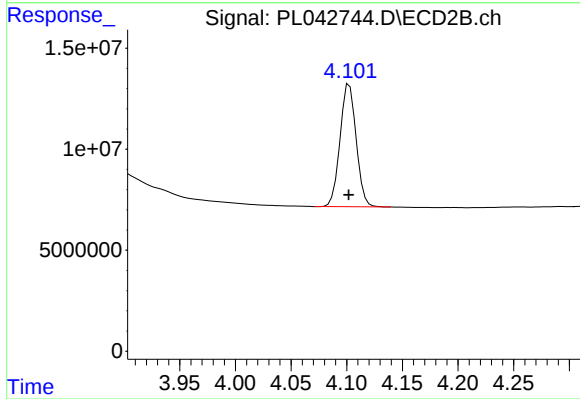


#1 Tetrachloro-m-xylene

R.T.: 4.102 min
Delta R.T.: 0.000 min
Response: 61239971
Conc: 21.29 ng/ml

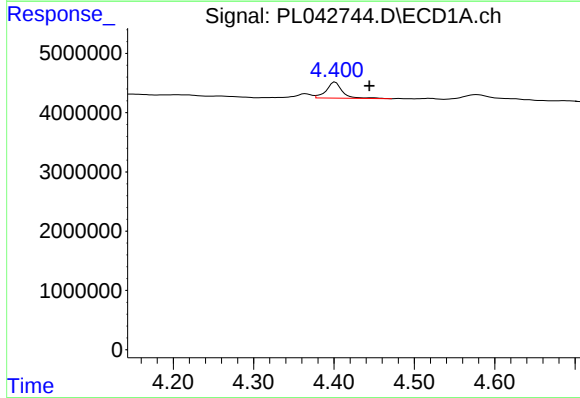


#6 beta-BHC

R.T.: 4.402 min
Delta R.T.: -0.043 min
Response: 3848861
Conc: 1.09 ng/ml

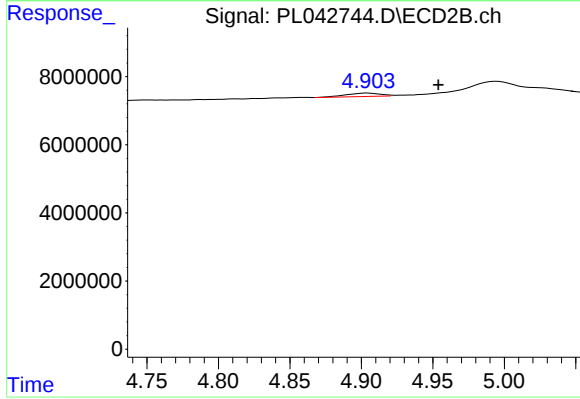

#6 beta-BHC


R.T.: 4.905 min
Delta R.T.: -0.049 min
Response: 1704411
Conc: 1.08 ng/ml

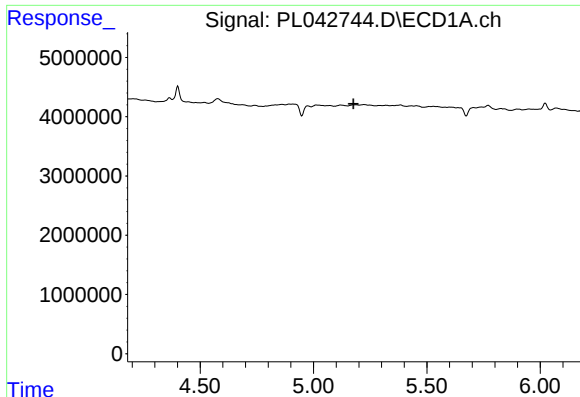

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.177 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

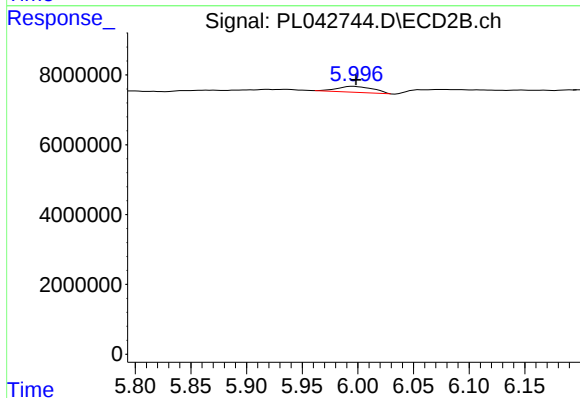


#8 Heptachlor epoxide

R.T.: 5.996 min
Delta R.T.: -0.002 min
Response: 3716490
Conc: 1.04 ng/ml

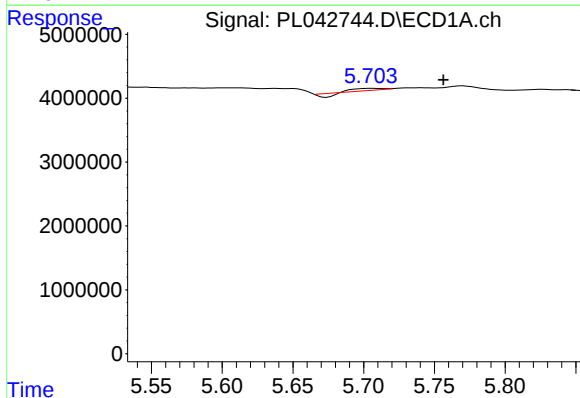


#13 Dieldrin

R.T.: 5.706 min
Delta R.T.: -0.051 min
Response: 200364
Conc: 0.03 ng/ml

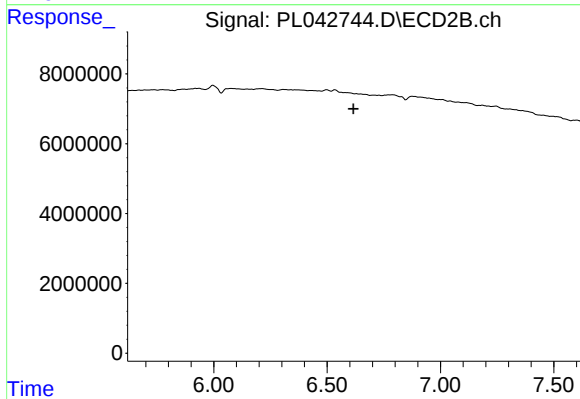

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.617 min
Response: 0
Conc: N.D.

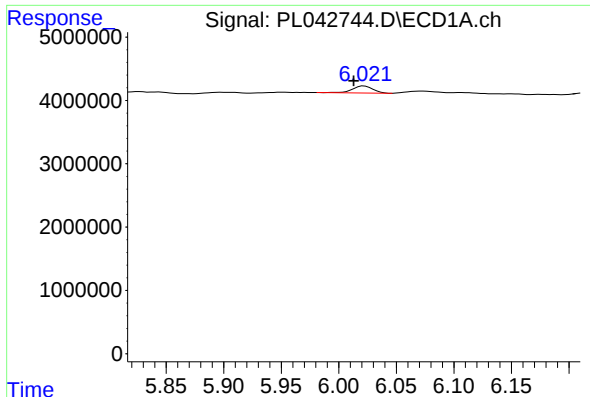

#14 Endrin


R.T.: 6.022 min
Delta R.T.: 0.009 min
Response: 1358991
Conc: 0.21 ng/ml

Instrument :
ECD_O
ClientSampleId :

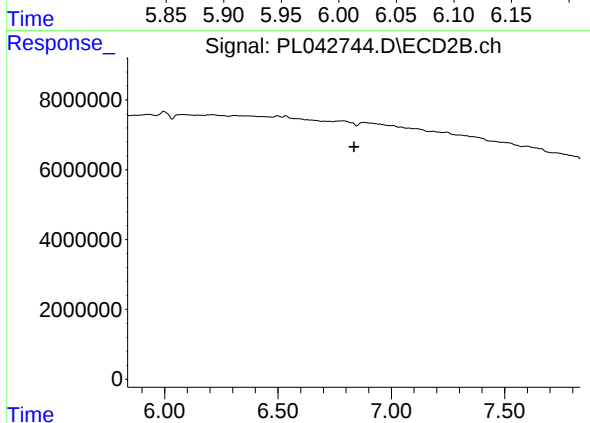


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.836 min
Response: 0
Conc: N.D.

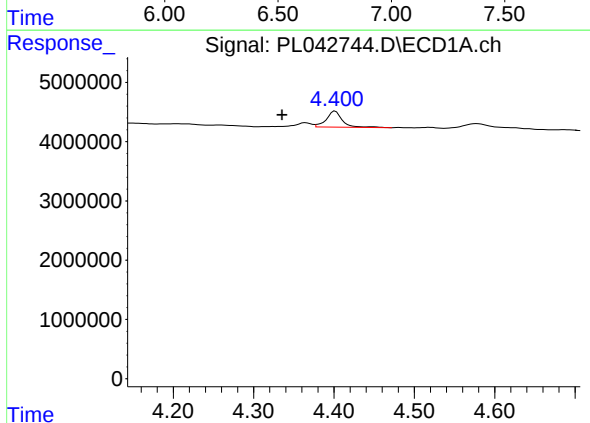


#23 Chlordane-1

R.T.: 4.402 min
Delta R.T.: 0.066 min
Response: 3848861
Conc: 13.92 ng/ml

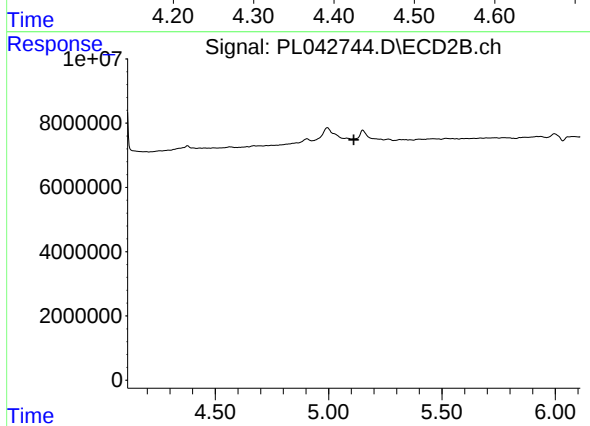

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.111 min
Response: 0
Conc: N.D.

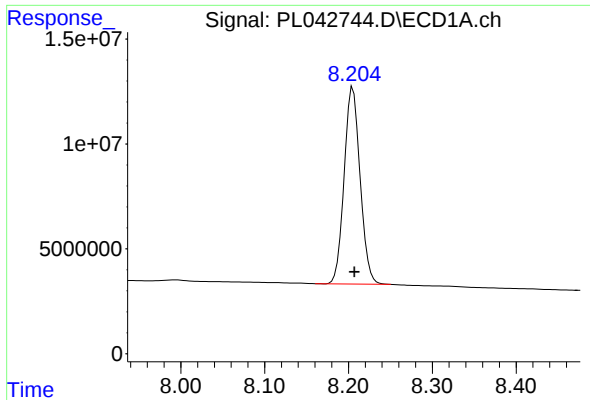

#28 Decachlorobiphenyl

R.T.: 8.205 min
Delta R.T.: -0.002 min
Response: 124308559
Conc: 19.72 ng/ml

Instrument :
ECD_O
ClientSampleId :

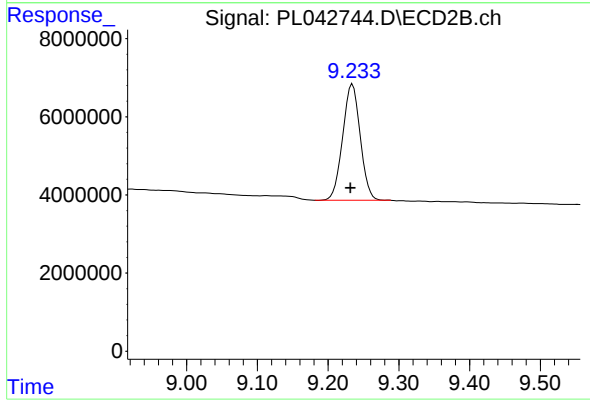

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.003 min
Response: 51372426
Conc: 21.30 ng/ml