

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120318\
Data File : PO052172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2018 20:19
Operator : SM/SJ
Sample : PB115247BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:17:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.282	3.296	16847600	4068213	19.569	18.241
2) SA Decachlor...	9.865	7.998	8841650	3756741	17.667	18.020

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120318\
Data File : PO052172.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2018 20:19
Operator : SM/SJ
Sample : PB115247BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:17:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

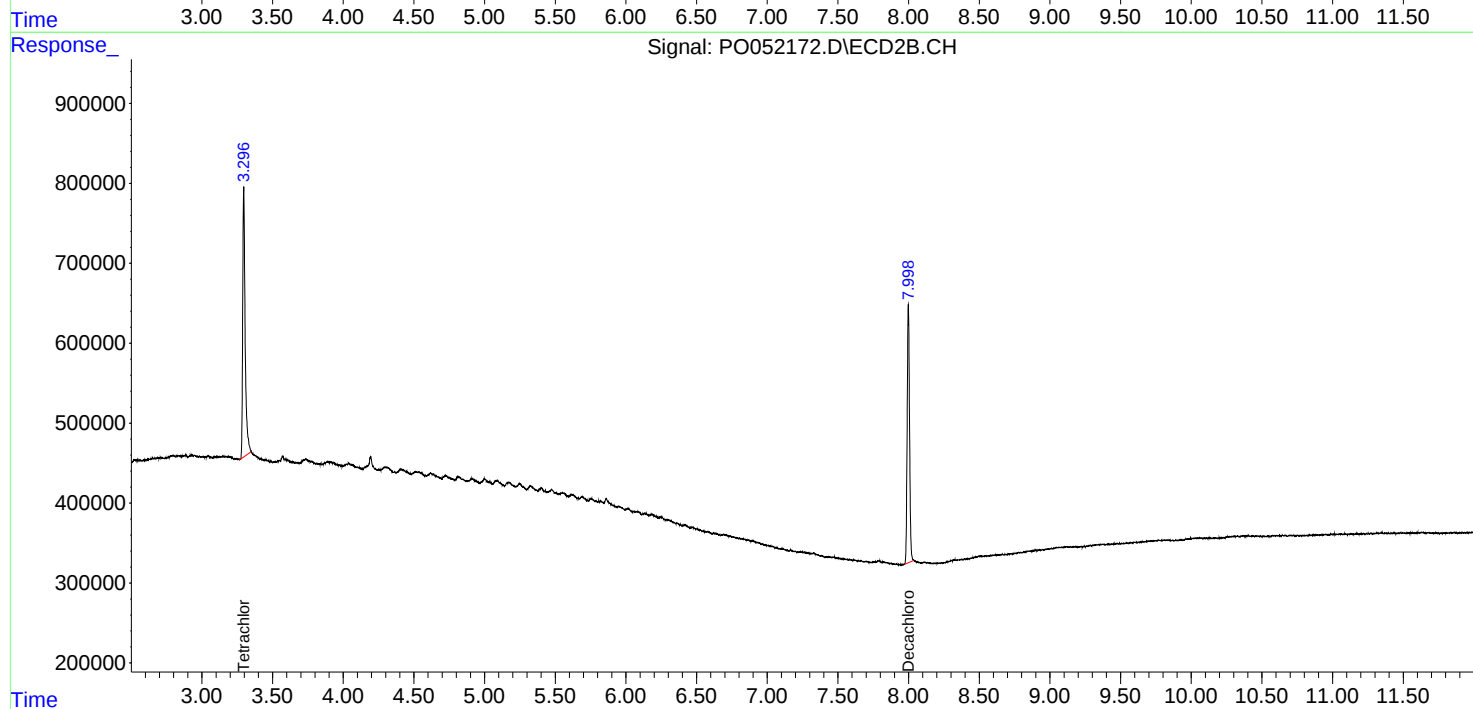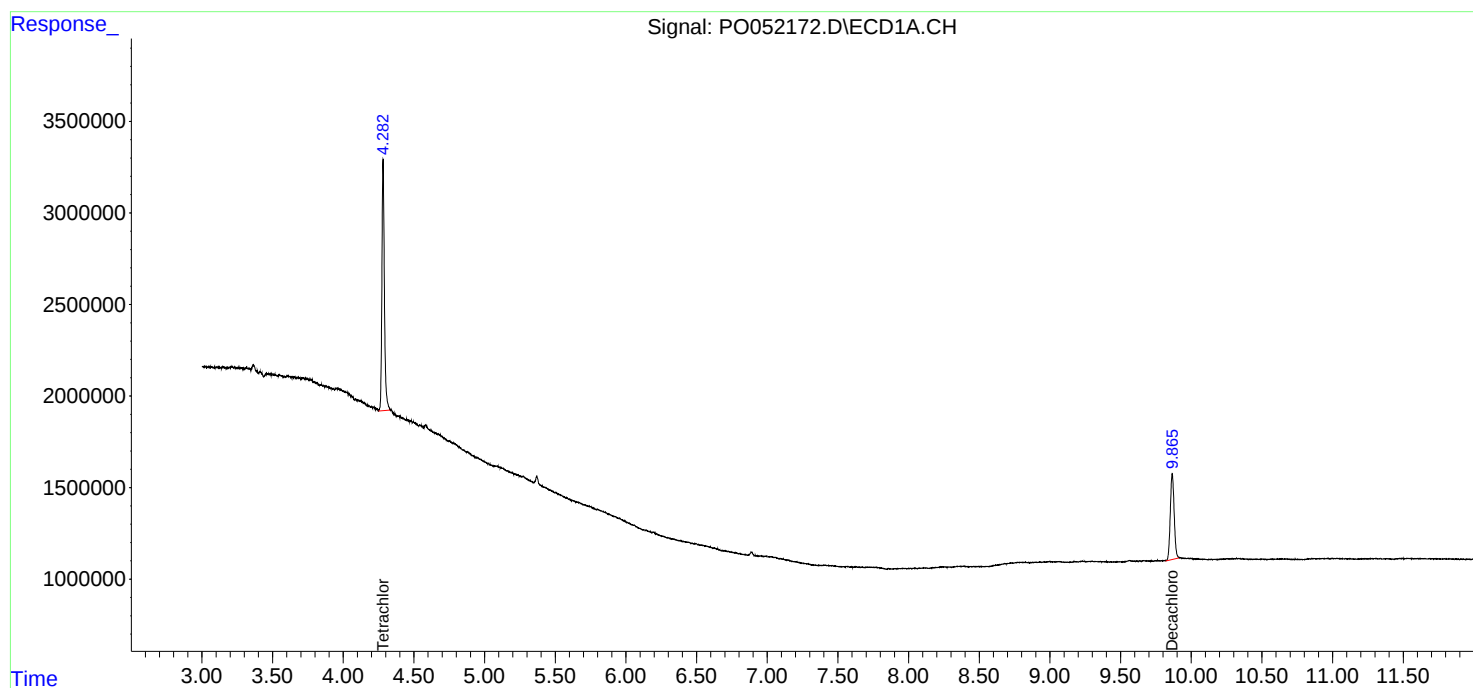


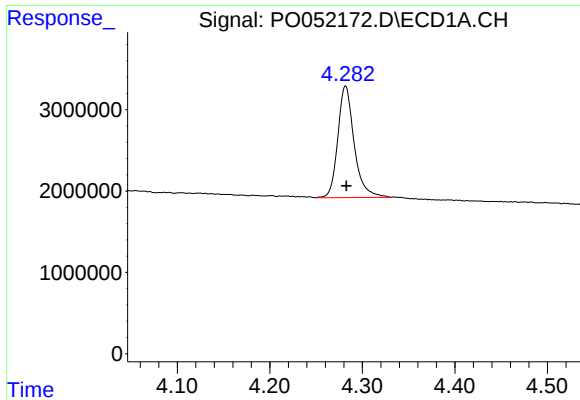

#1 Tetrachloro-m-xylene


R.T.: 4.282 min
Delta R.T.: -0.001 min
Response: 16847600
Conc: 19.57 ng/ml

Instrument :
ECD_O
ClientSampleId :

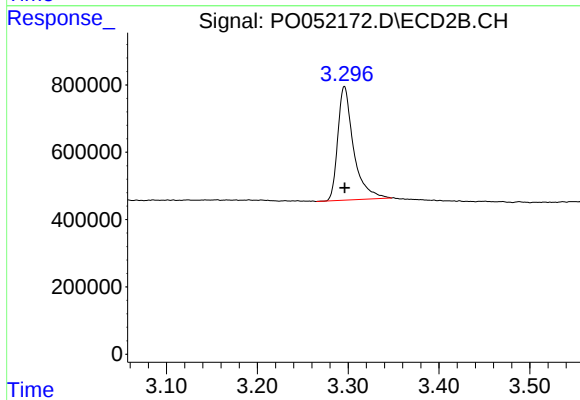


#1 Tetrachloro-m-xylene

R.T.: 3.296 min
Delta R.T.: 0.000 min
Response: 4068213
Conc: 18.24 ng/ml

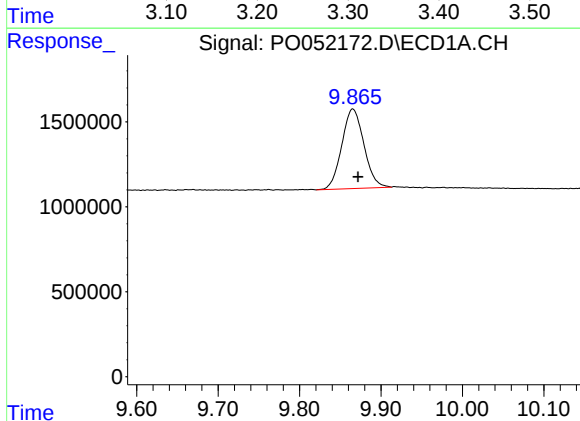

#2 Decachlorobiphenyl

R.T.: 9.865 min
Delta R.T.: -0.006 min
Response: 8841650
Conc: 17.67 ng/ml

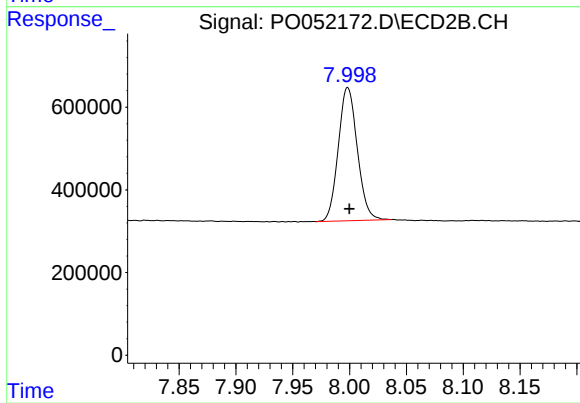

#2 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: -0.002 min
Response: 3756741
Conc: 18.02 ng/ml