

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120318\
Data File : PO052189.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2018 1:06
Operator : SM/SJ
Sample : J6153-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:28:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.283	3.297	21336901	5510265	24.784	24.706
2) SA Decachlor...	9.865	7.998	8652161	3827749	17.289	18.361

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120318\
Data File : PO052189.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2018 1:06
Operator : SM/SJ
Sample : J6153-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:28:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

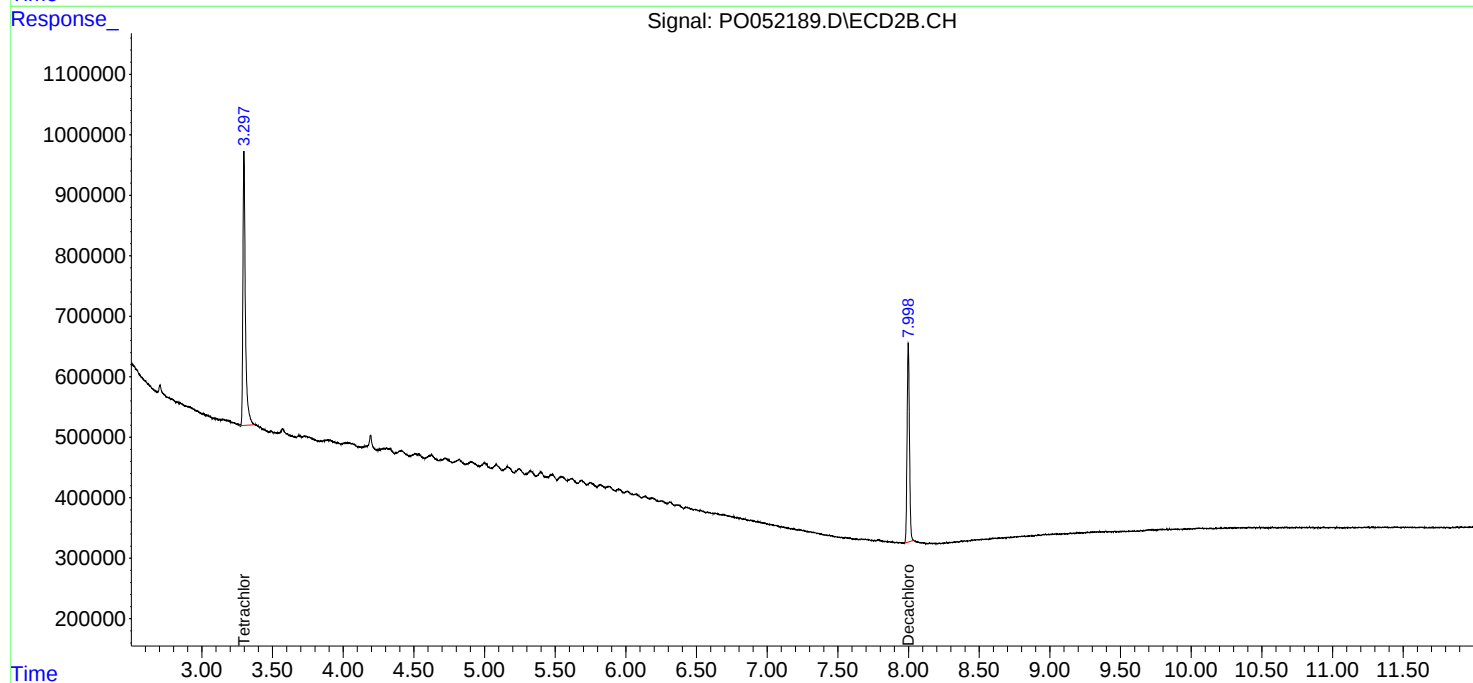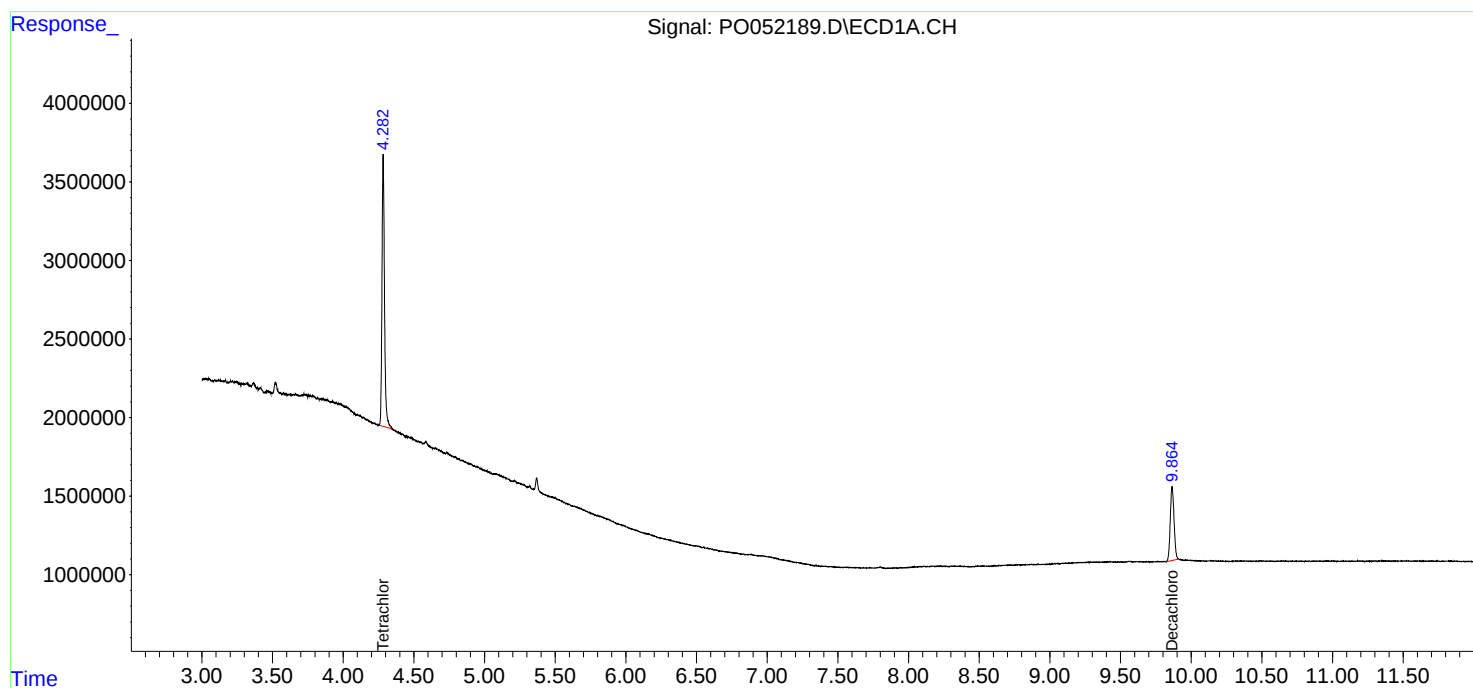


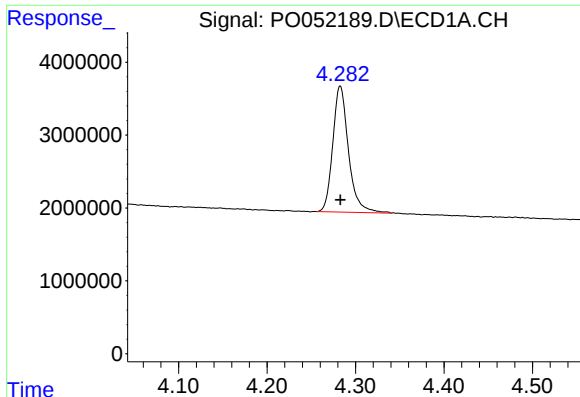

#1 Tetrachloro-m-xylene


R.T.: 4.283 min
Delta R.T.: 0.000 min
Response: 21336901
Conc: 24.78 ng/ml

Instrument :
ECD_O
ClientSampleId :

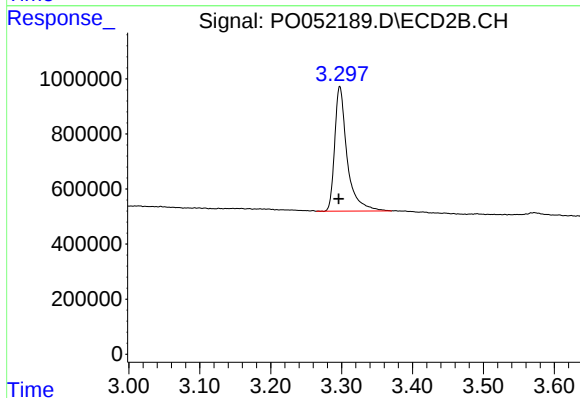


#1 Tetrachloro-m-xylene

R.T.: 3.297 min
Delta R.T.: 0.001 min
Response: 5510265
Conc: 24.71 ng/ml

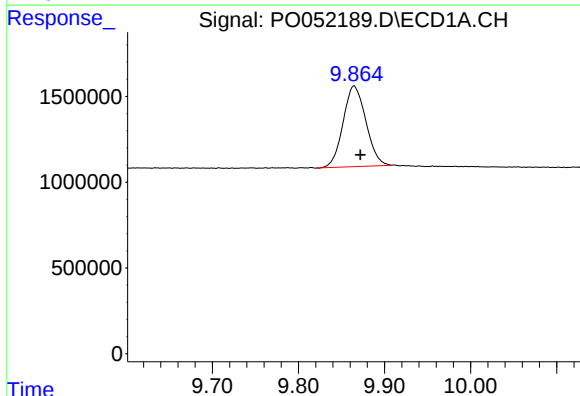

#2 Decachlorobiphenyl

R.T.: 9.865 min
Delta R.T.: -0.007 min
Response: 8652161
Conc: 17.29 ng/ml

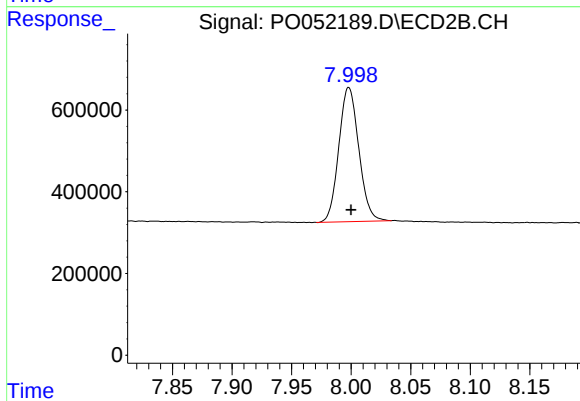

#2 Decachlorobiphenyl

R.T.: 7.998 min
Delta R.T.: -0.002 min
Response: 3827749
Conc: 18.36 ng/ml