

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120318\
 Data File : P0052158.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 03 Dec 2018 16:09
 Operator : SM/SJ
 Sample : J6160-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TEST-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 04:09:54 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.295	3.297	14036384	3250249	16.304	14.573
2) SA Decachlor...	9.888	8.004	6233911	2796591	12.457	13.415

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120318\
Data File : PO052158.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Dec 2018 16:09
Operator : SM/SJ
Sample : J6160-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TEST-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 04:09:54 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

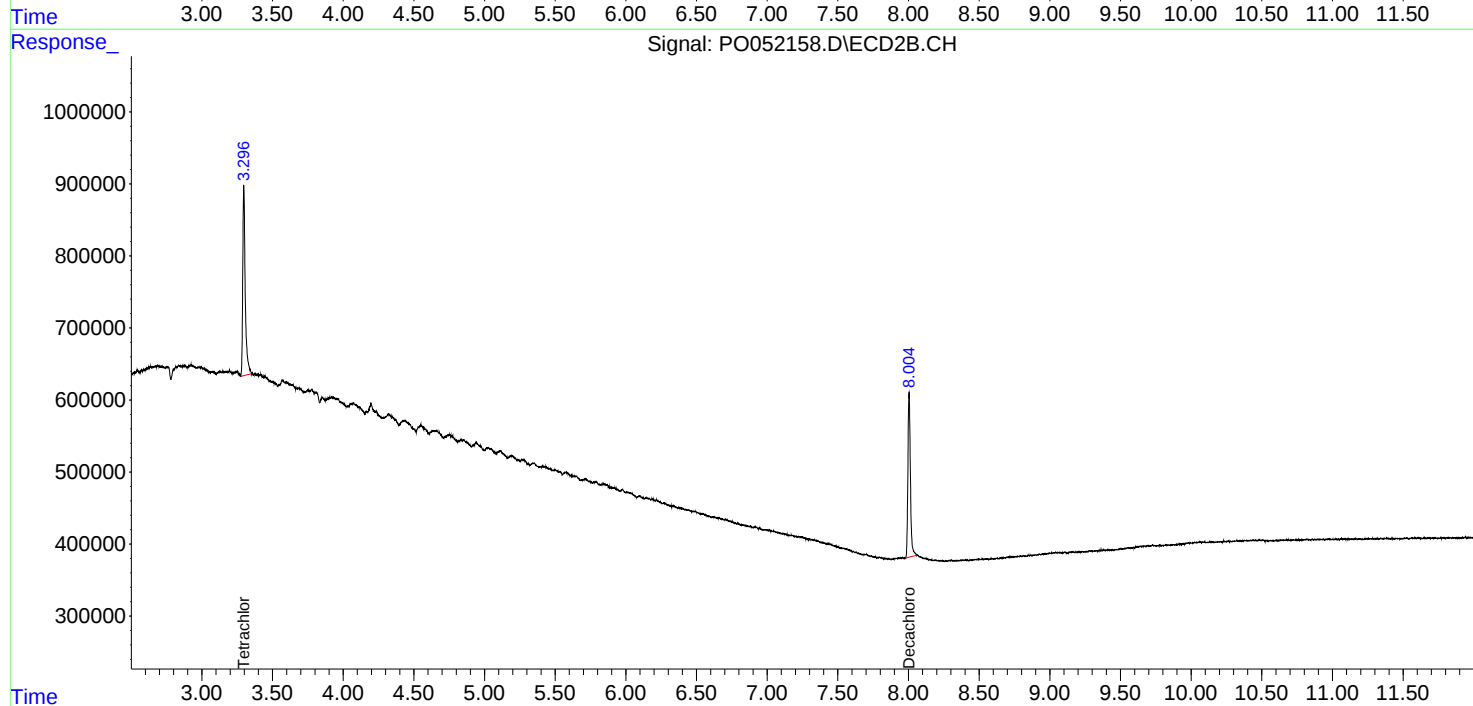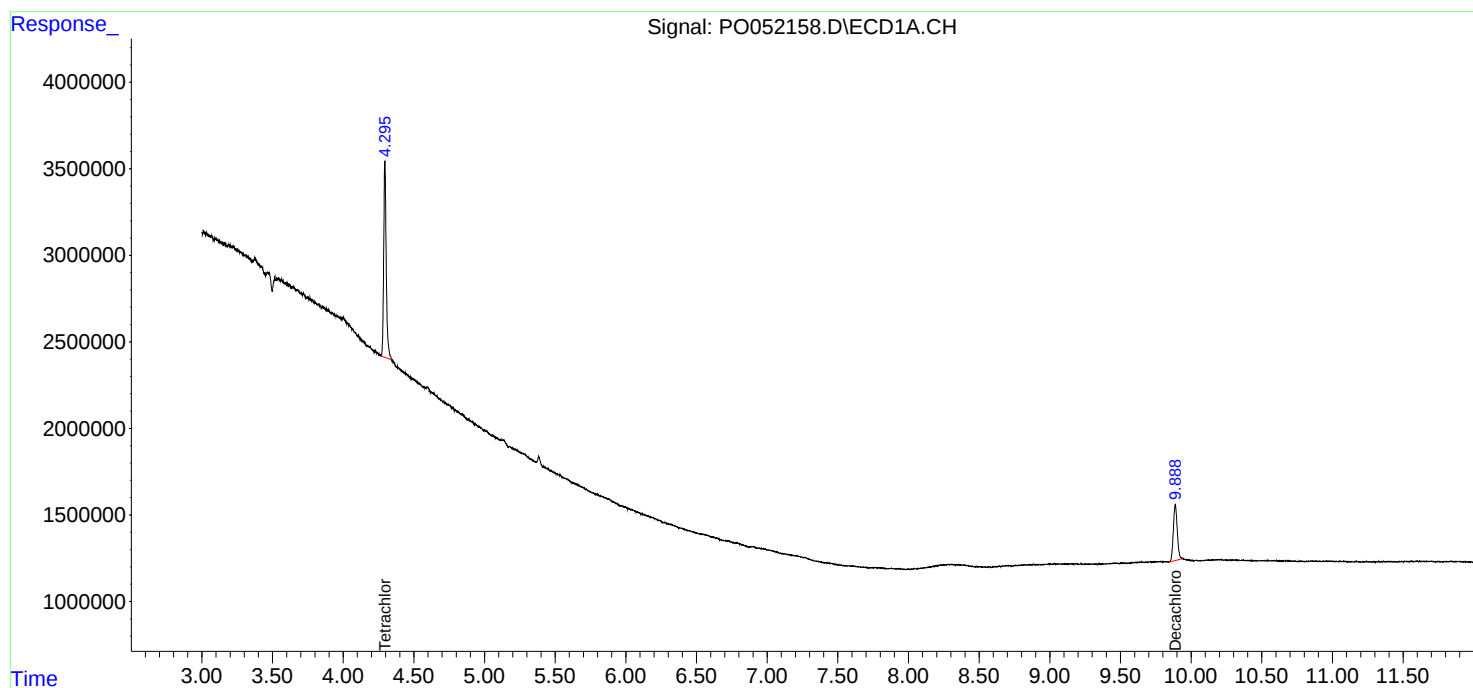


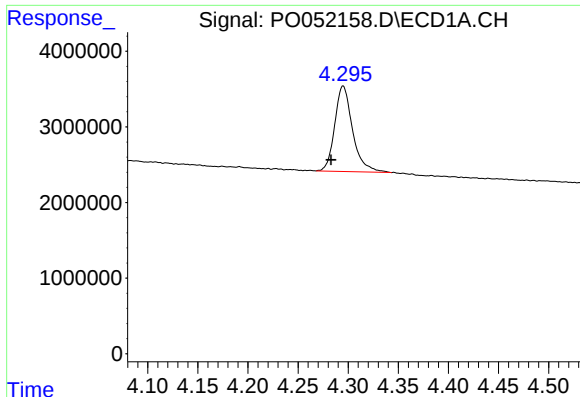

#1 Tetrachloro-m-xylene


R.T.: 4.295 min
Delta R.T.: 0.012 min
Response: 14036384
Conc: 16.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
TEST-PIT

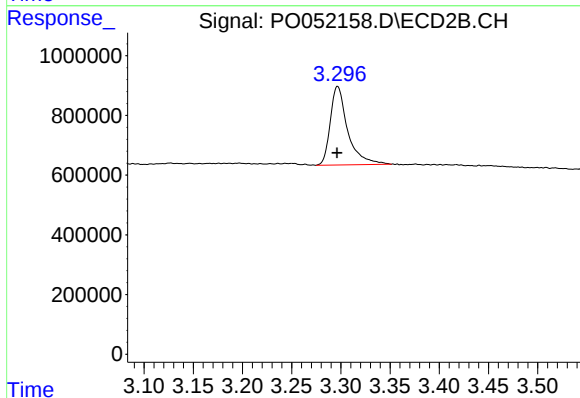


#1 Tetrachloro-m-xylene

R.T.: 3.297 min
Delta R.T.: 0.000 min
Response: 3250249
Conc: 14.57 ng/ml

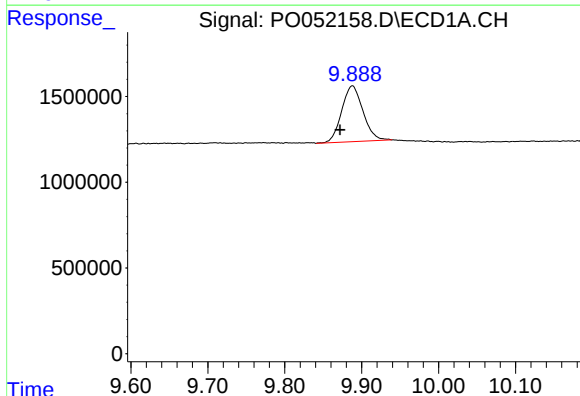

#2 Decachlorobiphenyl

R.T.: 9.888 min
Delta R.T.: 0.016 min
Response: 6233911
Conc: 12.46 ng/ml

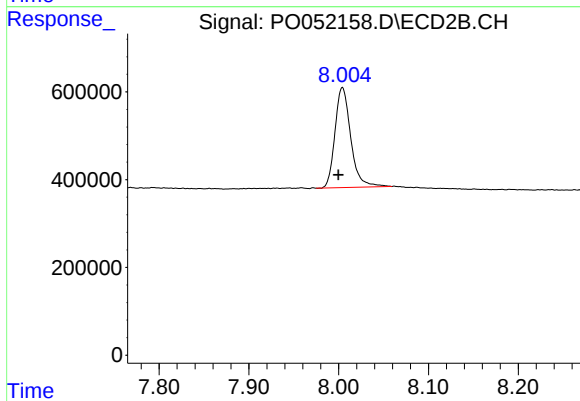

#2 Decachlorobiphenyl

R.T.: 8.004 min
Delta R.T.: 0.004 min
Response: 2796591
Conc: 13.41 ng/ml