

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120418\
 Data File : P0052221.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2018 12:00
 Operator : SM/SJ
 Sample : J6179-09
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S9-0-0.5-BGS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 12:15:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.277	3.292	15047024	4102809	17.478	18.396
2) SA Decachlor...	9.858	7.992	6780279	3069573	13.548	14.724

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120418\
Data File : PO052221.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2018 12:00
Operator : SM/SJ
Sample : J6179-09
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S9-0-0.5-BGS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 12:15:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

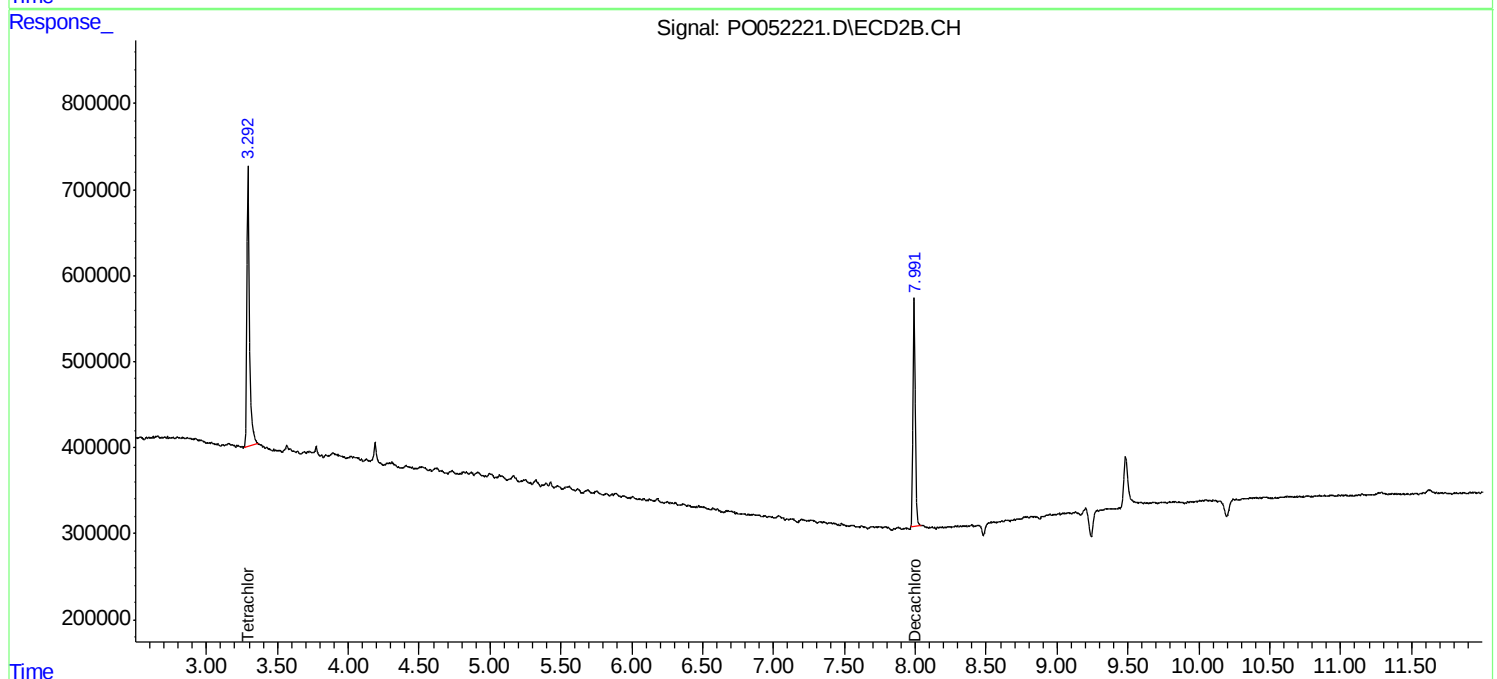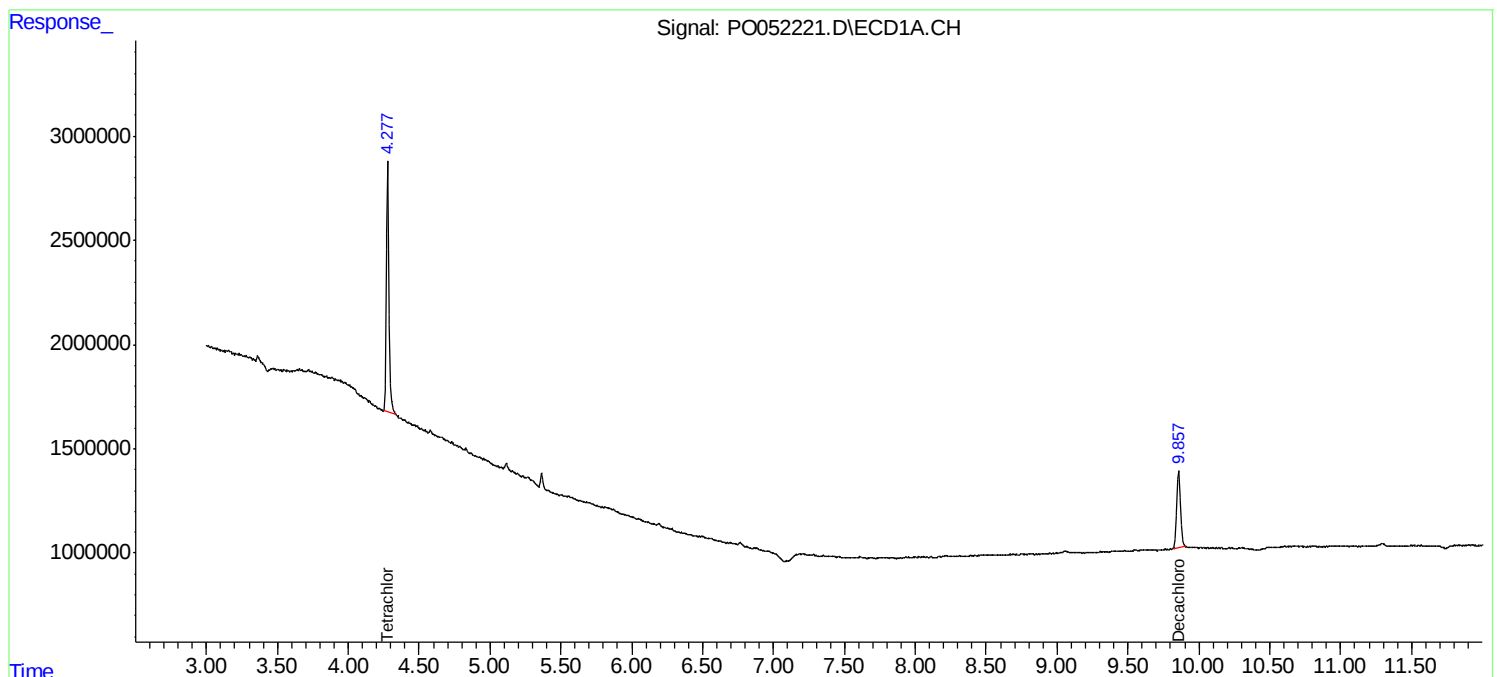


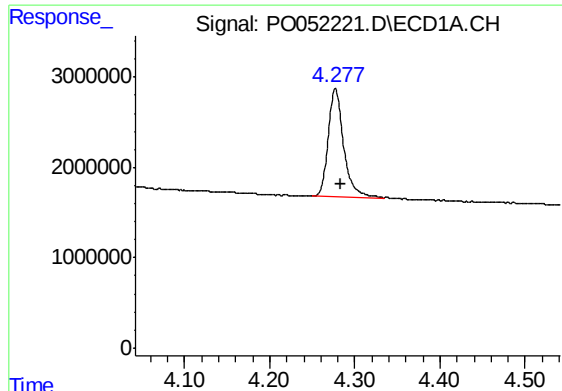

#1 Tetrachloro-m-xylene


R.T.: 4.277 min
Delta R.T.: -0.006 min
Response: 15047024
Conc: 17.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
S9-0-0.5-BGS

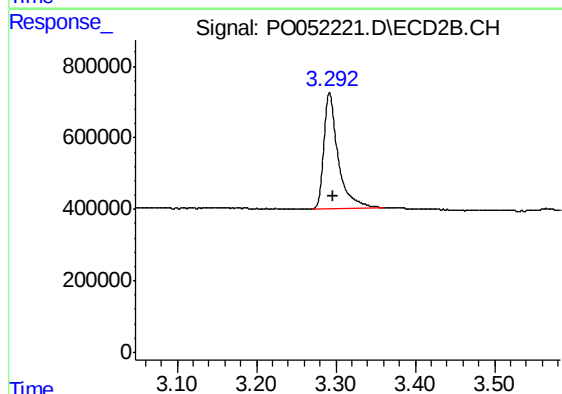


#1 Tetrachloro-m-xylene

R.T.: 3.292 min
Delta R.T.: -0.004 min
Response: 4102809
Conc: 18.40 ng/ml

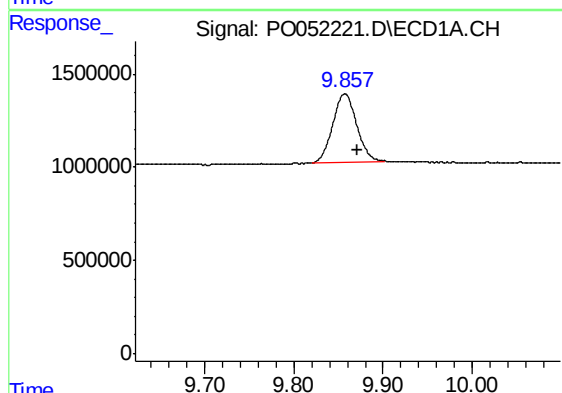

#2 Decachlorobiphenyl

R.T.: 9.858 min
Delta R.T.: -0.014 min
Response: 6780279
Conc: 13.55 ng/ml

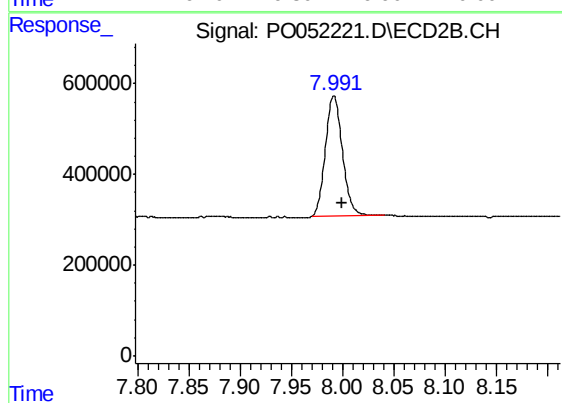

#2 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.008 min
Response: 3069573
Conc: 14.72 ng/ml