

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120418\
 Data File : P0052225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Dec 2018 13:08
 Operator : SM/SJ
 Sample : J6179-07RE
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 S7-0-0.5-BGSRE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 04 13:35:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.278	3.292	14290691	3775717	16.599	16.929
2)	SA Decachlor...	9.856	7.992	5258251	2374757	10.507	11.391

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120418\
Data File : PO052225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Dec 2018 13:08
Operator : SM/SJ
Sample : J6179-07RE
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
S7-0-0.5-BGSRE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 04 13:35:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

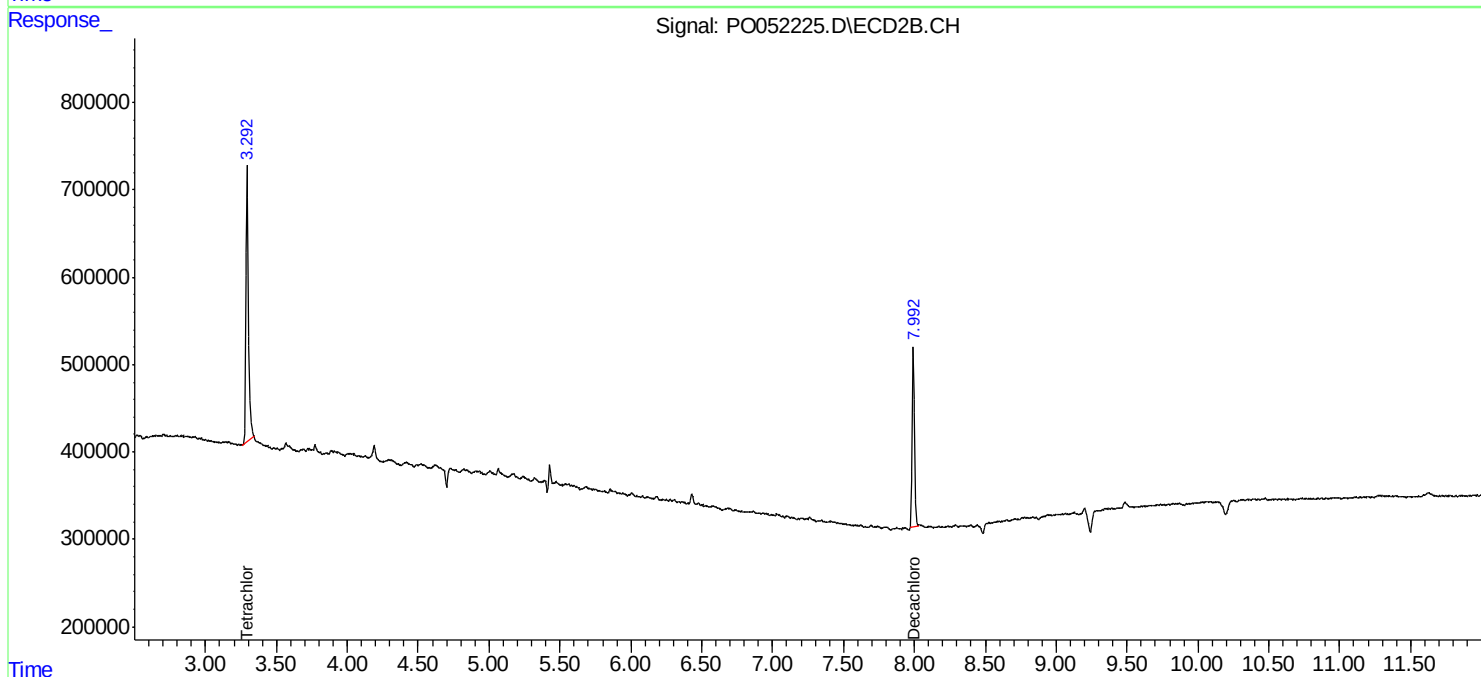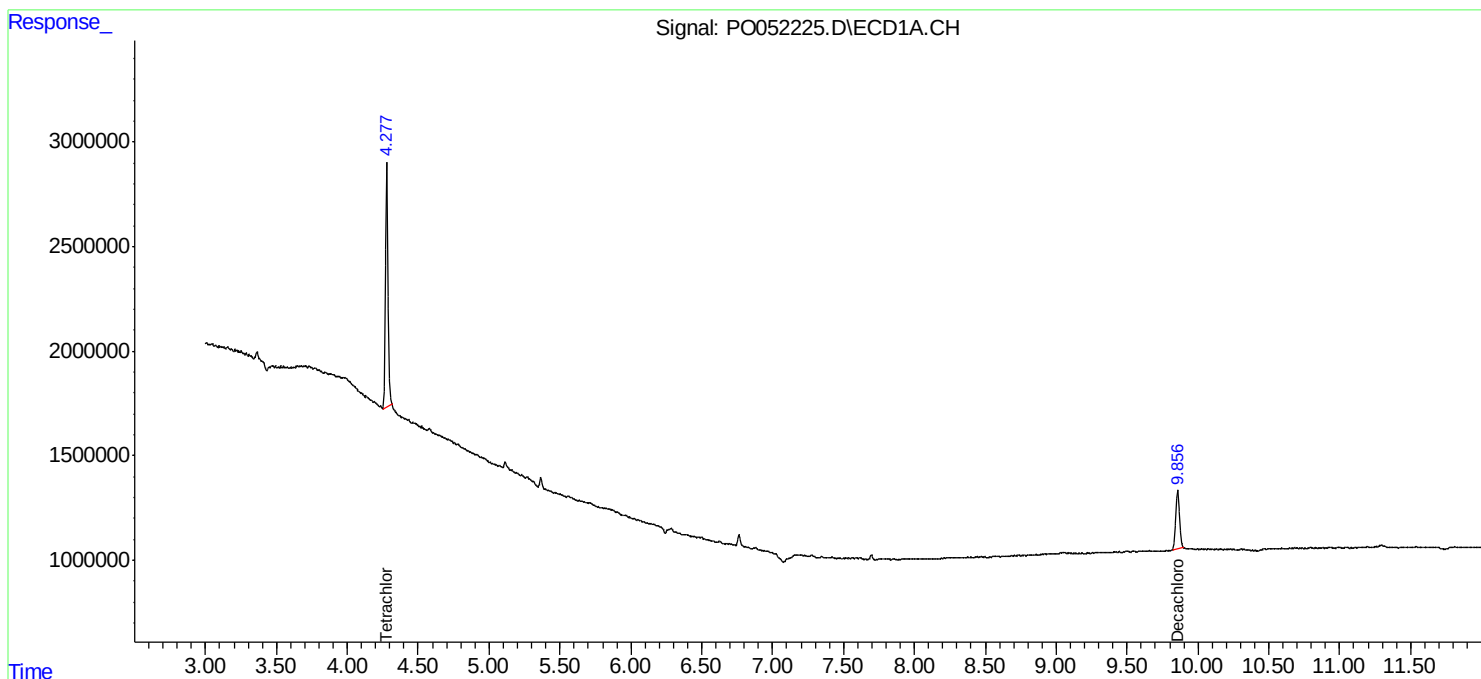


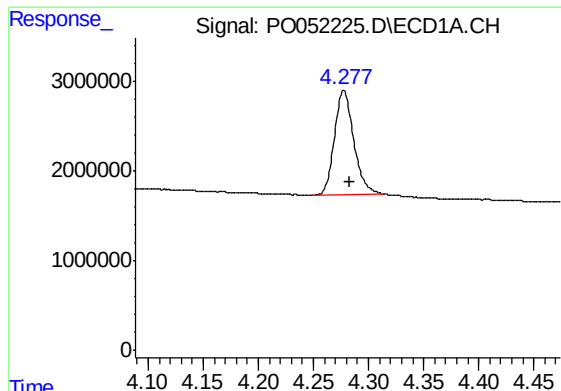

#1 Tetrachloro-m-xylene


R.T.: 4.278 min
Delta R.T.: -0.005 min
Response: 14290691
Conc: 16.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
S7-0-0.5-BGSRE

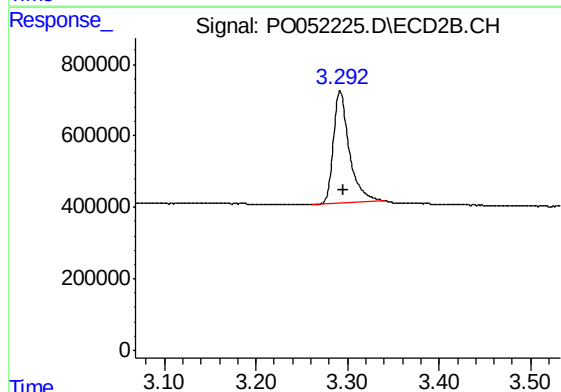


#1 Tetrachloro-m-xylene

R.T.: 3.292 min
Delta R.T.: -0.004 min
Response: 3775717
Conc: 16.93 ng/ml

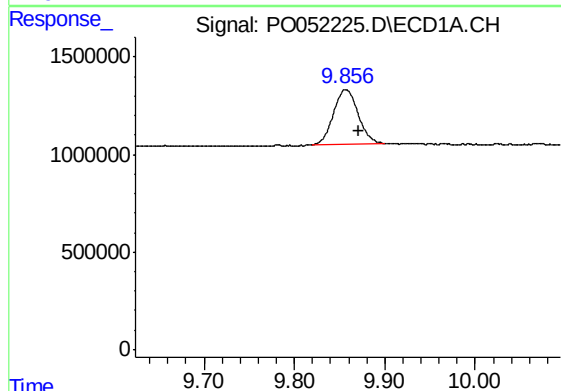

#2 Decachlorobiphenyl

R.T.: 9.856 min
Delta R.T.: -0.015 min
Response: 5258251
Conc: 10.51 ng/ml

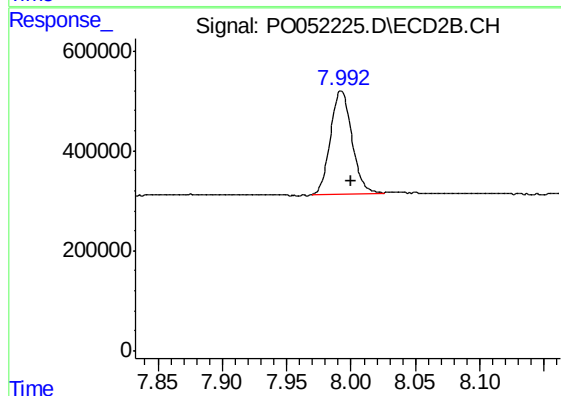

#2 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: -0.008 min
Response: 2374757
Conc: 11.39 ng/ml