

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120718\
Data File : PO052349.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2018 00:01
Operator : SM/SJ
Sample : PB115429BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 02:03:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.271	3.288	18115294	4784068	21.042	21.450
2) SA Decachlor...	9.837	7.980	9956578	4505448	19.895	21.612

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120718\
Data File : PO052349.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Dec 2018 00:01
Operator : SM/SJ
Sample : PB115429BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 02:03:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

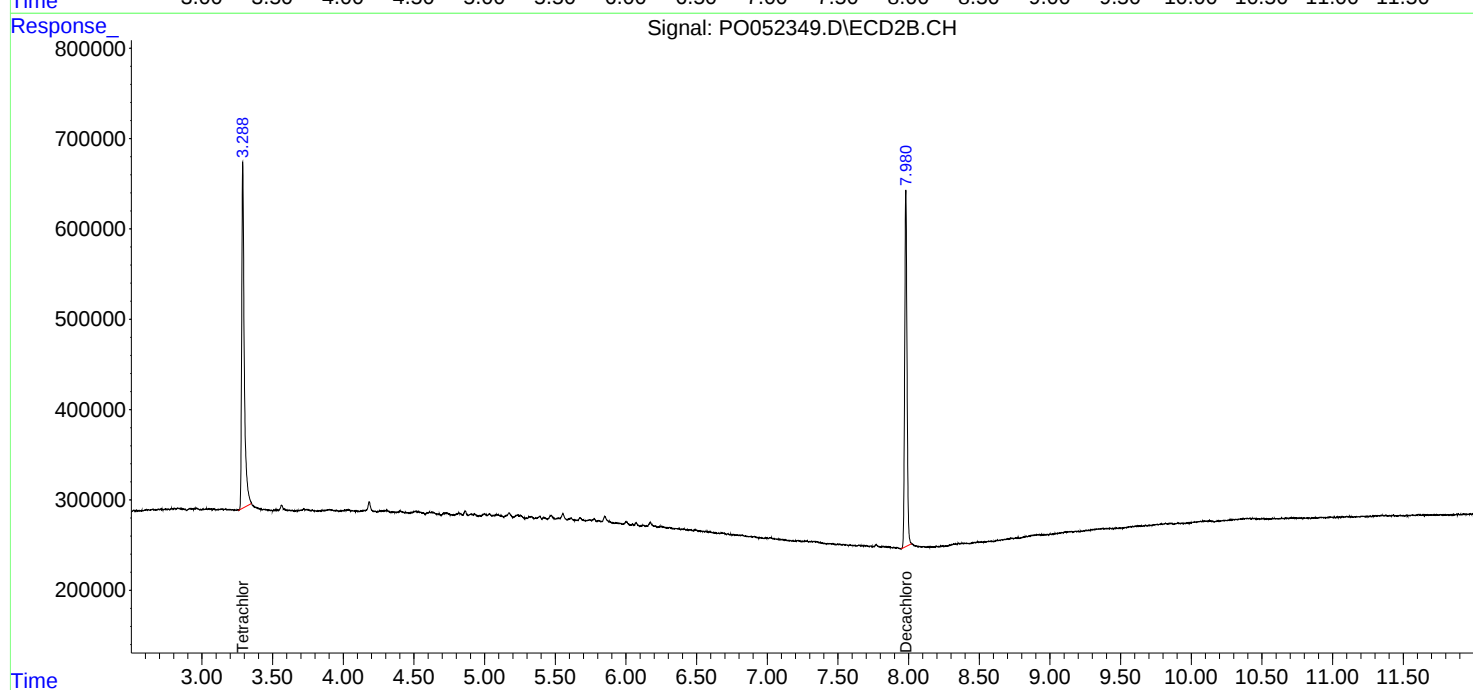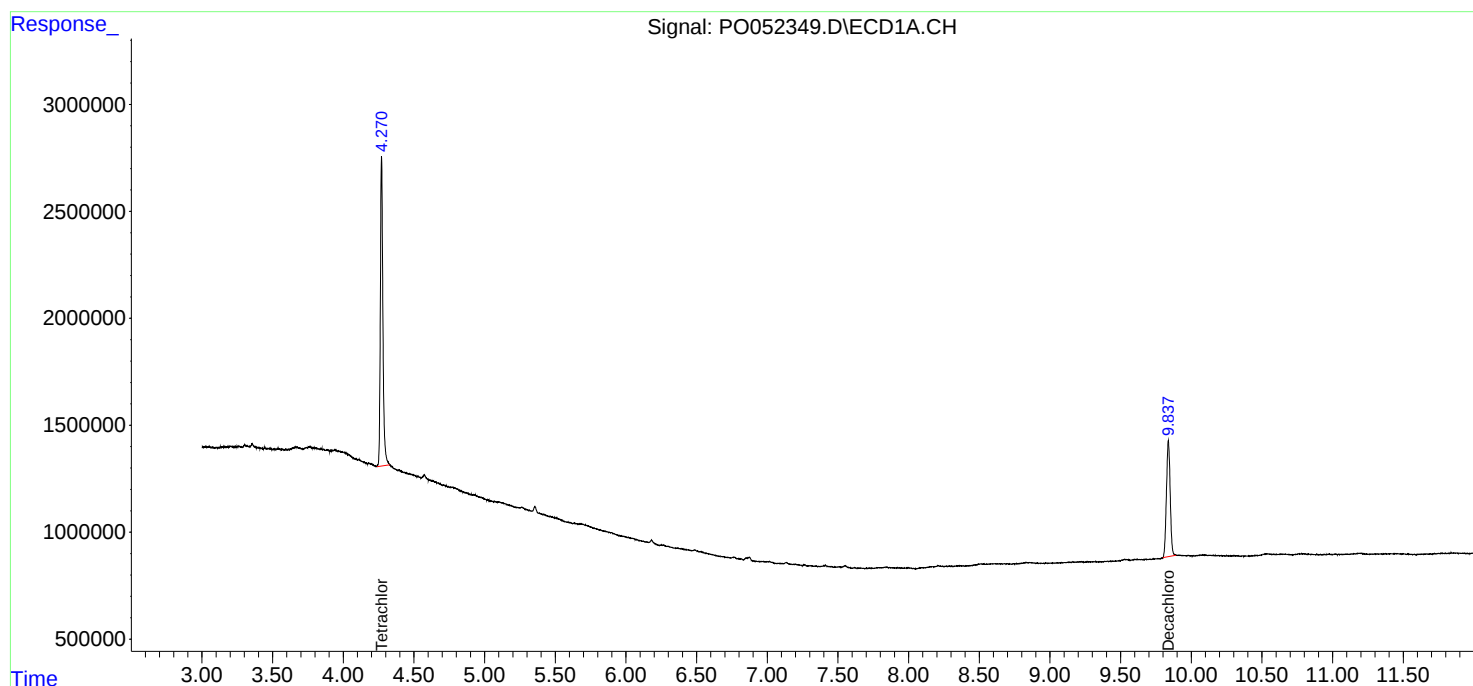


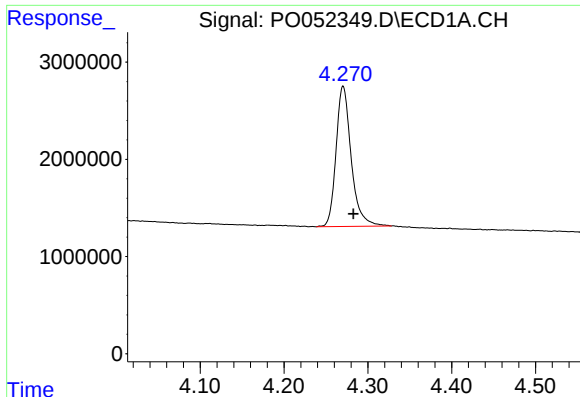

#1 Tetrachloro-m-xylene


R.T.: 4.271 min
Delta R.T.: -0.012 min
Response: 18115294
Conc: 21.04 ng/ml

Instrument :
ECD_O
ClientSampleId :

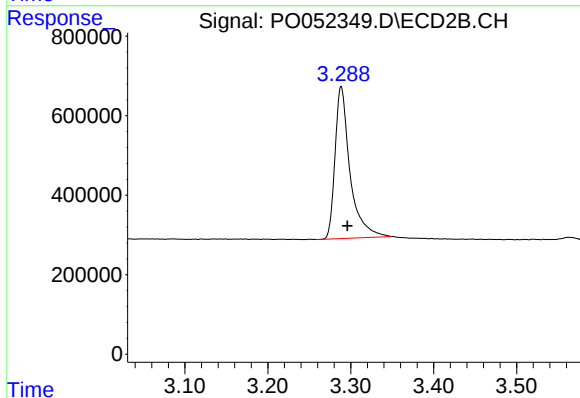


#1 Tetrachloro-m-xylene

R.T.: 3.288 min
Delta R.T.: -0.008 min
Response: 4784068
Conc: 21.45 ng/ml

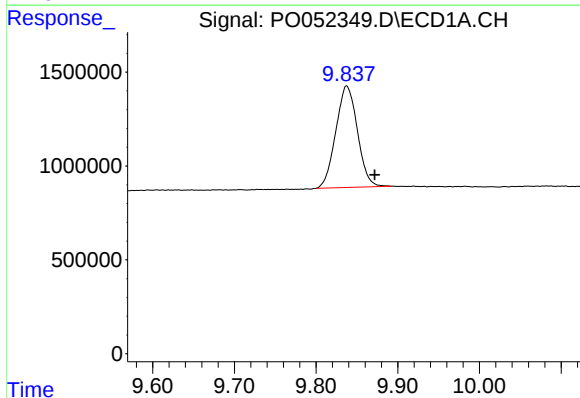

#2 Decachlorobiphenyl

R.T.: 9.837 min
Delta R.T.: -0.034 min
Response: 9956578
Conc: 19.90 ng/ml

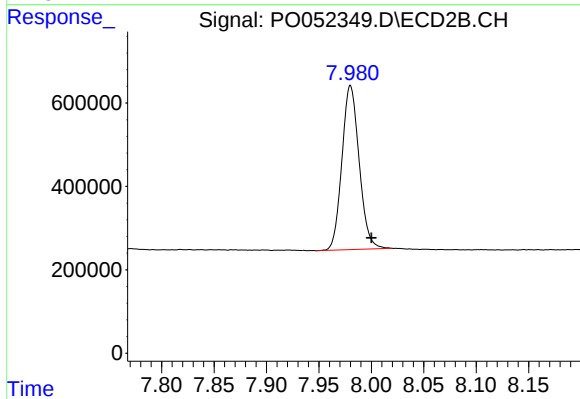

#2 Decachlorobiphenyl

R.T.: 7.980 min
Delta R.T.: -0.020 min
Response: 4505448
Conc: 21.61 ng/ml