

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120718\
 Data File : P0052326.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Dec 2018 16:34
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Sohil
 12/10/2018 2:20:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 21:58:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Dec 04 03:10:39 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.276	3.289	21146308	5393854	24.562	24.184
2)	SA Decachlor...	9.845	7.983	10119079	4580905	20.220m	21.974m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120718\
Data File : PO052326.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Dec 2018 16:34
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
12/10/2018 2:20:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 21:58:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO120318.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Dec 04 03:10:39 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

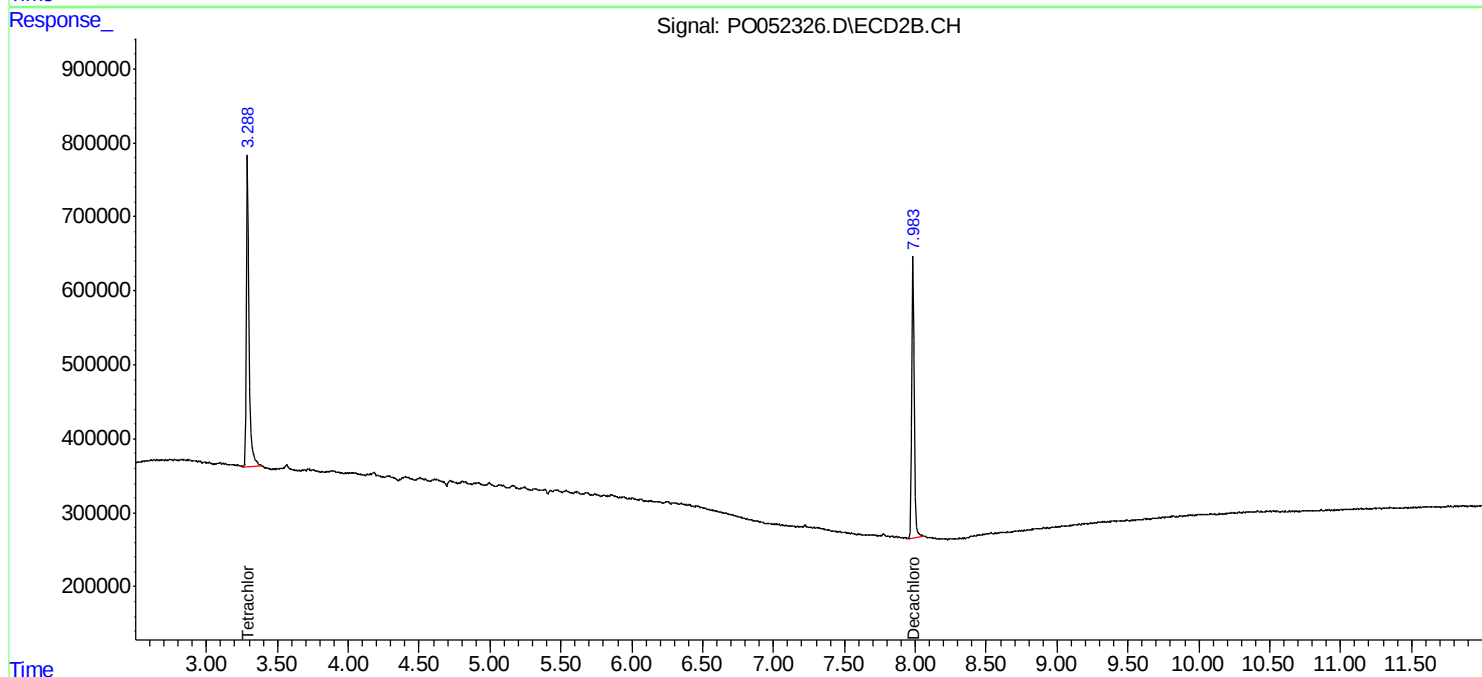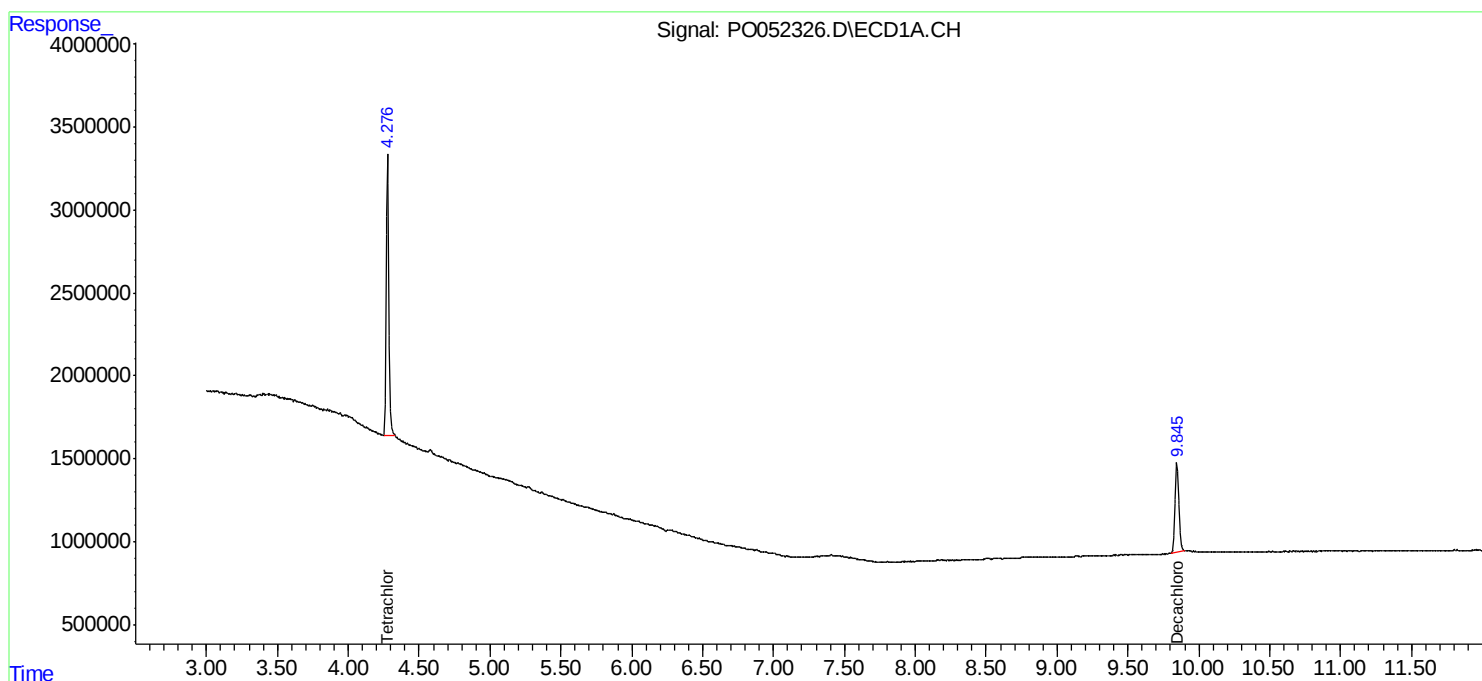

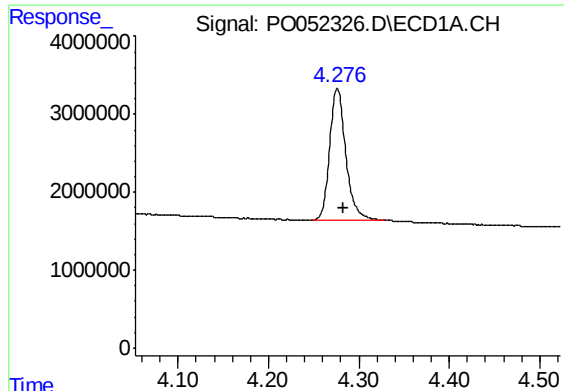


#1 Tetrachloro-m-xylene

R.T.: 4.276 min
Delta R.T.: -0.007 min
Response: 21146308
Conc: 24.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Sohil
12/10/2018 2:20:25 PM

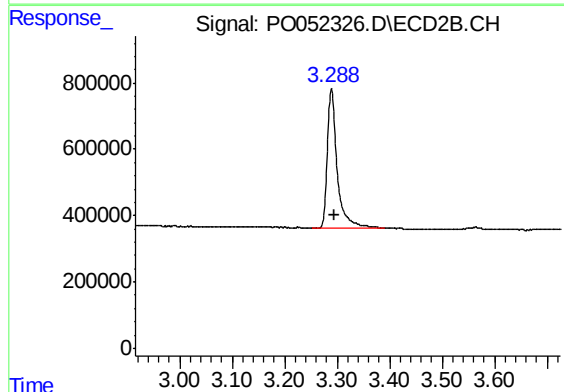


#1 Tetrachloro-m-xylene

R.T.: 3.289 min
Delta R.T.: -0.007 min
Response: 5393854
Conc: 24.18 ng/ml

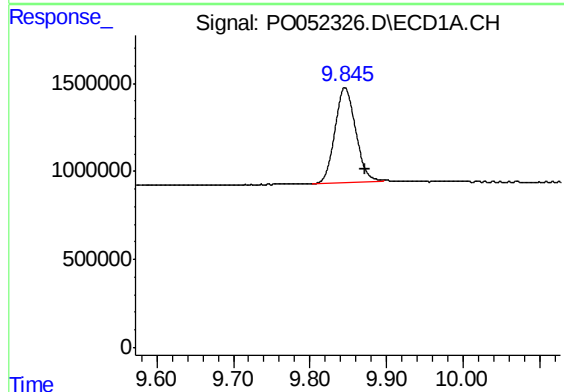

#2 Decachlorobiphenyl

R.T.: 9.845 min
Delta R.T.: -0.027 min
Response: 10119079
Conc: 20.22 ng/ml m

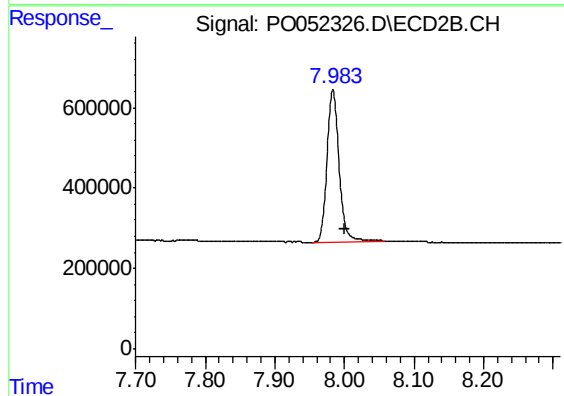

#2 Decachlorobiphenyl

R.T.: 7.983 min
Delta R.T.: -0.017 min
Response: 4580905
Conc: 21.97 ng/ml m