

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0120719\
 Data File : P0064464.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Dec 2019 8:35
 Operator : SM/AJ
 Sample : K6183-01RE 5X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 01-A-01-B-01-CRE

Manual Integrations
 APPROVED

mohammad
 12/9/2019 12:06:41 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 01:16:39 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.311	3.559	89068	64664	3.008m	2.719
2)	SA Decachlor...	9.933	8.515	97130	91748	2.370	2.246

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO120719\
Data File : PO064464.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Dec 2019 8:35
Operator : SM/AJ
Sample : K6183-01RE 5X
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-CRE


Manual Integrations
APPROVED

mohammad
12/9/2019 12:06:41 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 01:16:39 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

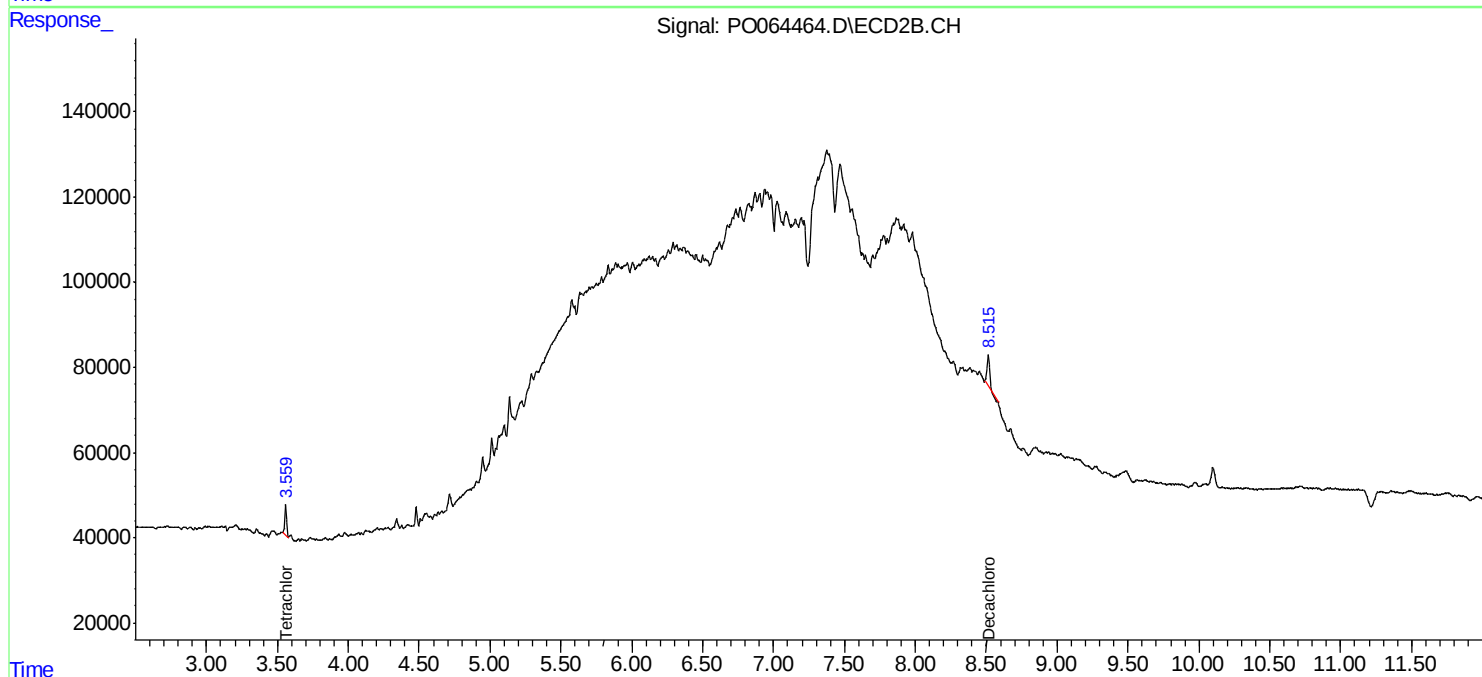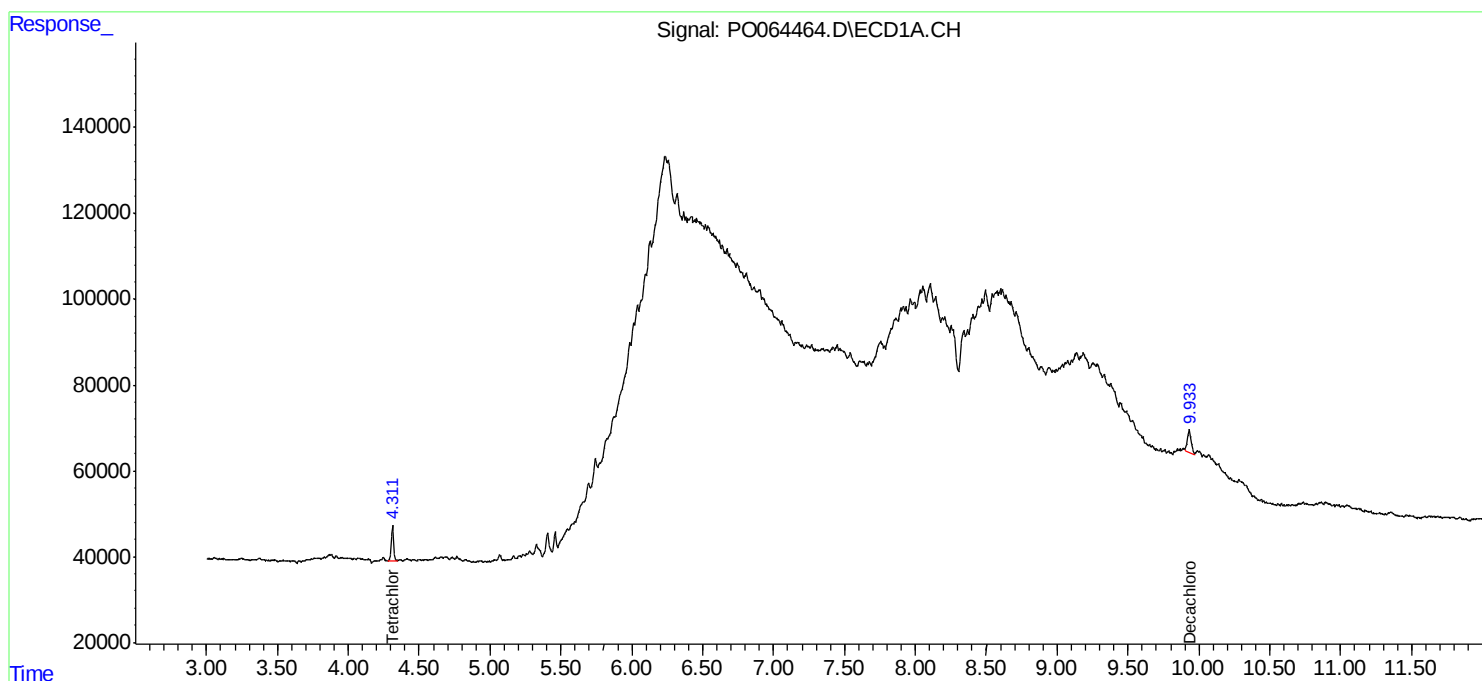

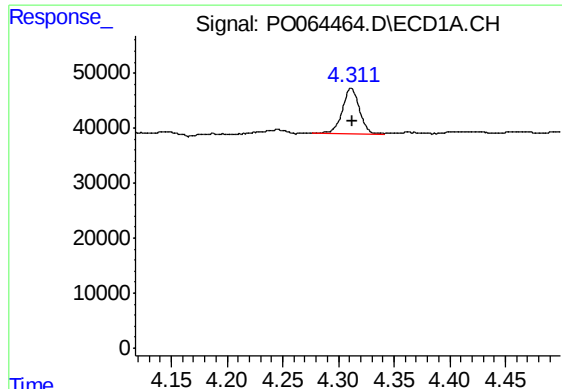


#1 Tetrachloro-m-xylene

R.T.: 4.311 min
Delta R.T.: -0.002 min
Response: 89068
Conc: 3.01 ng/ml m

Instrument :
ECD_O
ClientSampleId :
01-A-01-B-01-CRE


Manual Integrations
APPROVED

mohammad
12/9/2019 12:06:41 PM

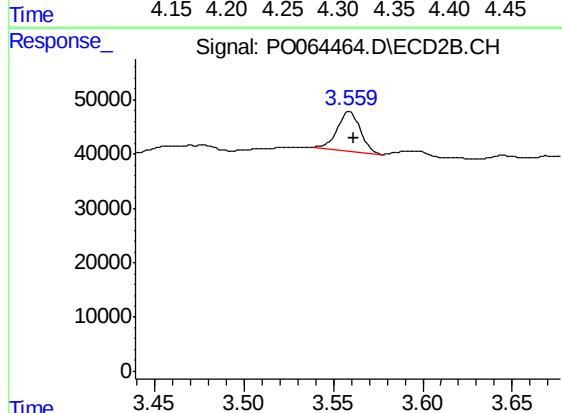


#1 Tetrachloro-m-xylene

R.T.: 3.559 min
Delta R.T.: -0.002 min
Response: 64664
Conc: 2.72 ng/ml

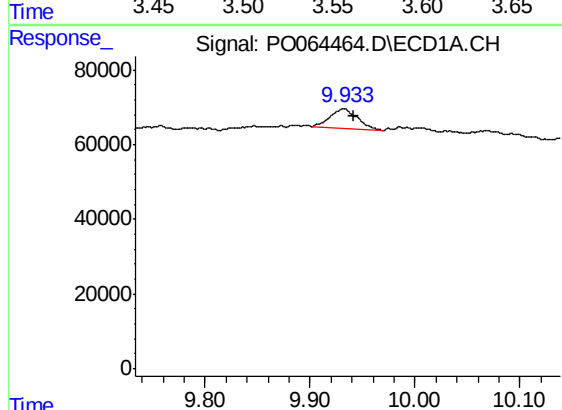

#2 Decachlorobiphenyl

R.T.: 9.933 min
Delta R.T.: -0.008 min
Response: 97130
Conc: 2.37 ng/ml

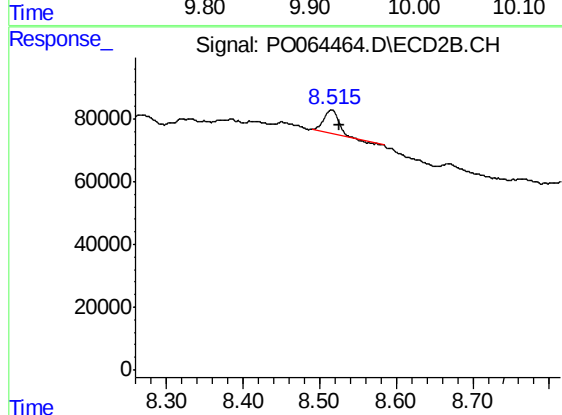

#2 Decachlorobiphenyl

R.T.: 8.515 min
Delta R.T.: -0.011 min
Response: 91748
Conc: 2.25 ng/ml