

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121019\
 Data File : P0064511.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Dec 2019 18:05
 Operator : SM/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 12/11/2019 1:08:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 05:28:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0112719.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 28 01:28:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.324	3.567	482213	427476	16.283m	17.972
2) SA Decachlor...	9.953	8.526	598898	694654	14.613	17.005

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121019\
Data File : PO064511.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Dec 2019 18:05
Operator : SM/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
12/11/2019 1:08:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 05:28:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO112719.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 28 01:28:08 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

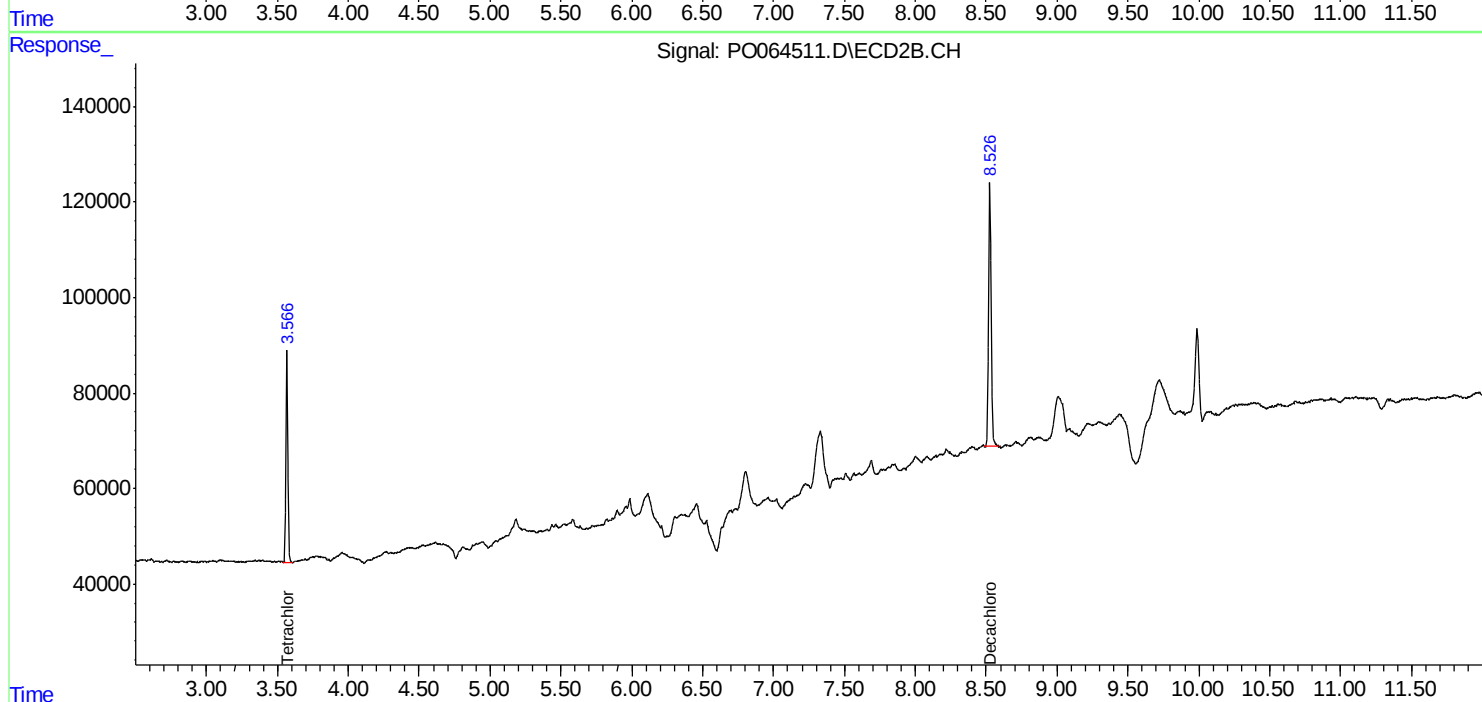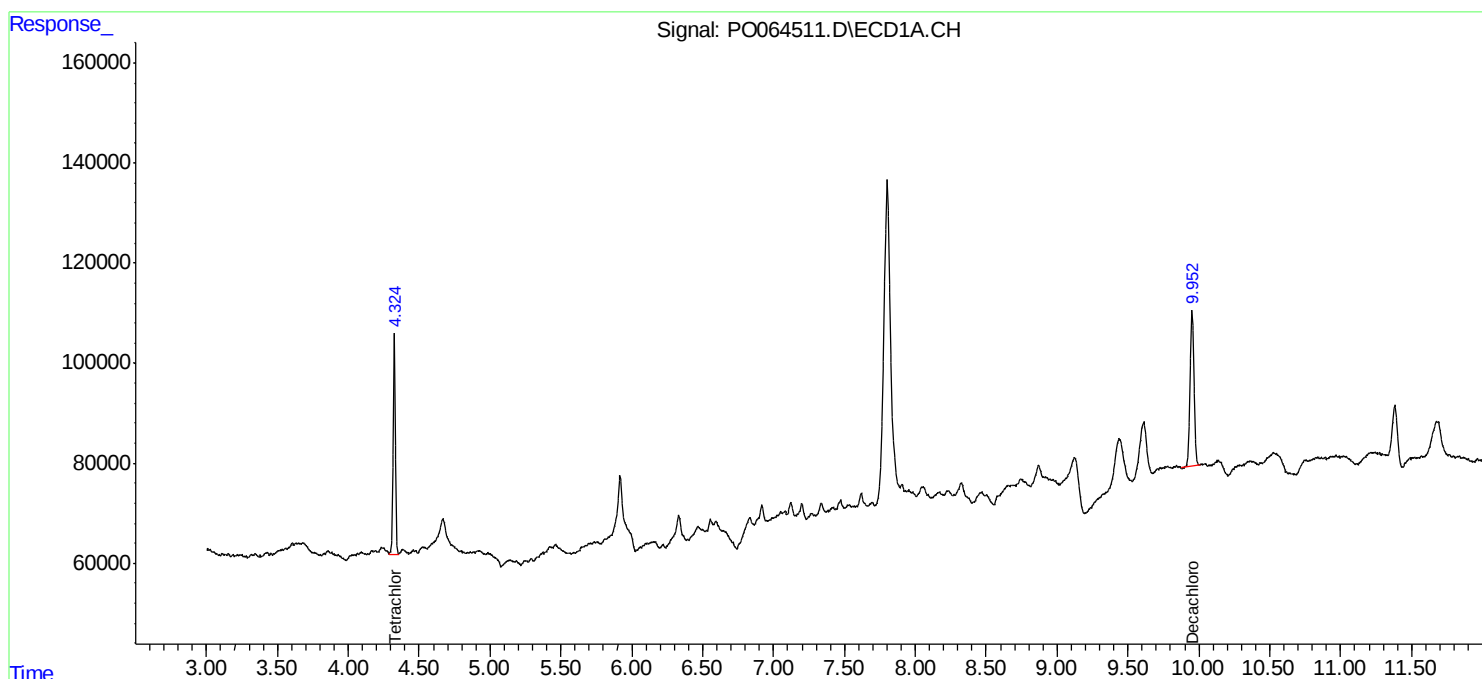

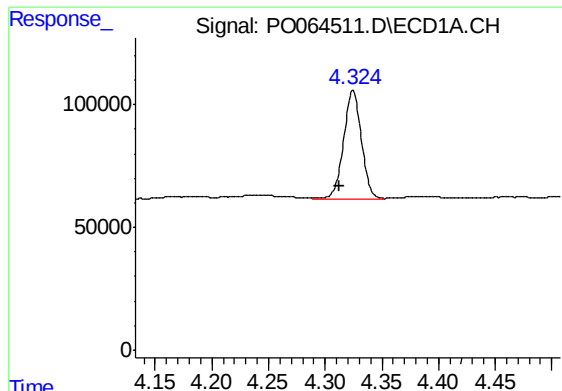


#1 Tetrachloro-m-xylene

R.T.: 4.324 min
Delta R.T.: 0.011 min
Response: 482213
Conc: 16.28 ng/ml m

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
12/11/2019 1:08:59 PM

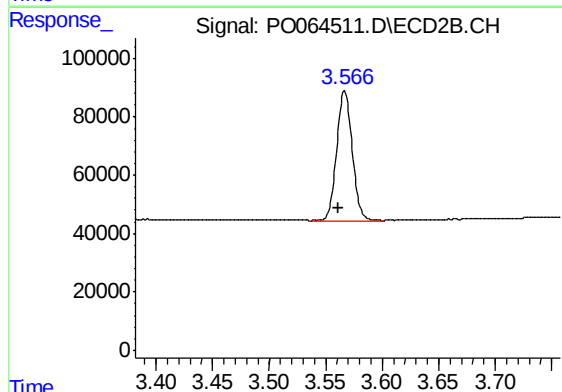


#1 Tetrachloro-m-xylene

R.T.: 3.567 min
Delta R.T.: 0.005 min
Response: 427476
Conc: 17.97 ng/ml

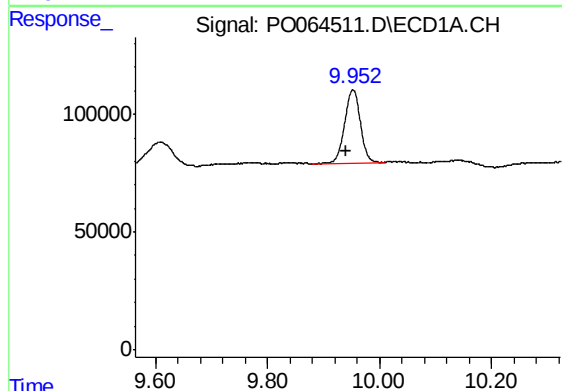

#2 Decachlorobiphenyl

R.T.: 9.953 min
Delta R.T.: 0.012 min
Response: 598898
Conc: 14.61 ng/ml

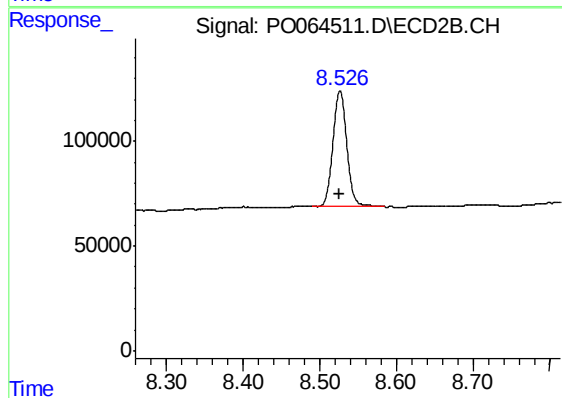

#2 Decachlorobiphenyl

R.T.: 8.526 min
Delta R.T.: 0.000 min
Response: 694654
Conc: 17.00 ng/ml