

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121419\
 Data File : P0064606.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Dec 2019 12:06
 Operator : SM/AJ
 Sample : K6265-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TP-1A-S

Manual Integrations
 APPROVED

Ankita
 12/16/2019 10:09:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 13:02:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.179	3.458	661440	778711	27.169m	30.719m
2)	SA Decachlor...	9.690	8.379	601917	702061	19.613m	20.216

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121419\
Data File : PO064606.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Dec 2019 12:06
Operator : SM/AJ
Sample : K6265-03
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TP-1A-S


Manual Integrations
APPROVED

Ankita
12/16/2019 10:09:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 13:02:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

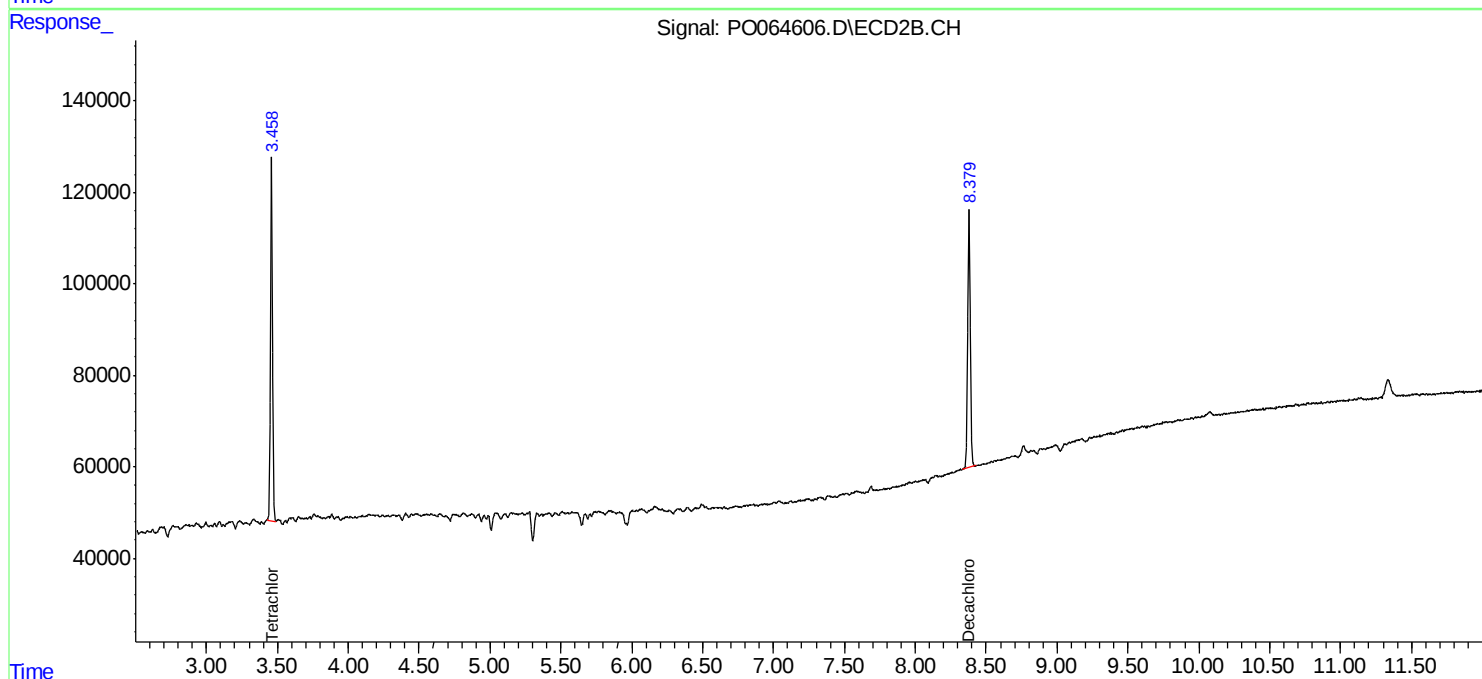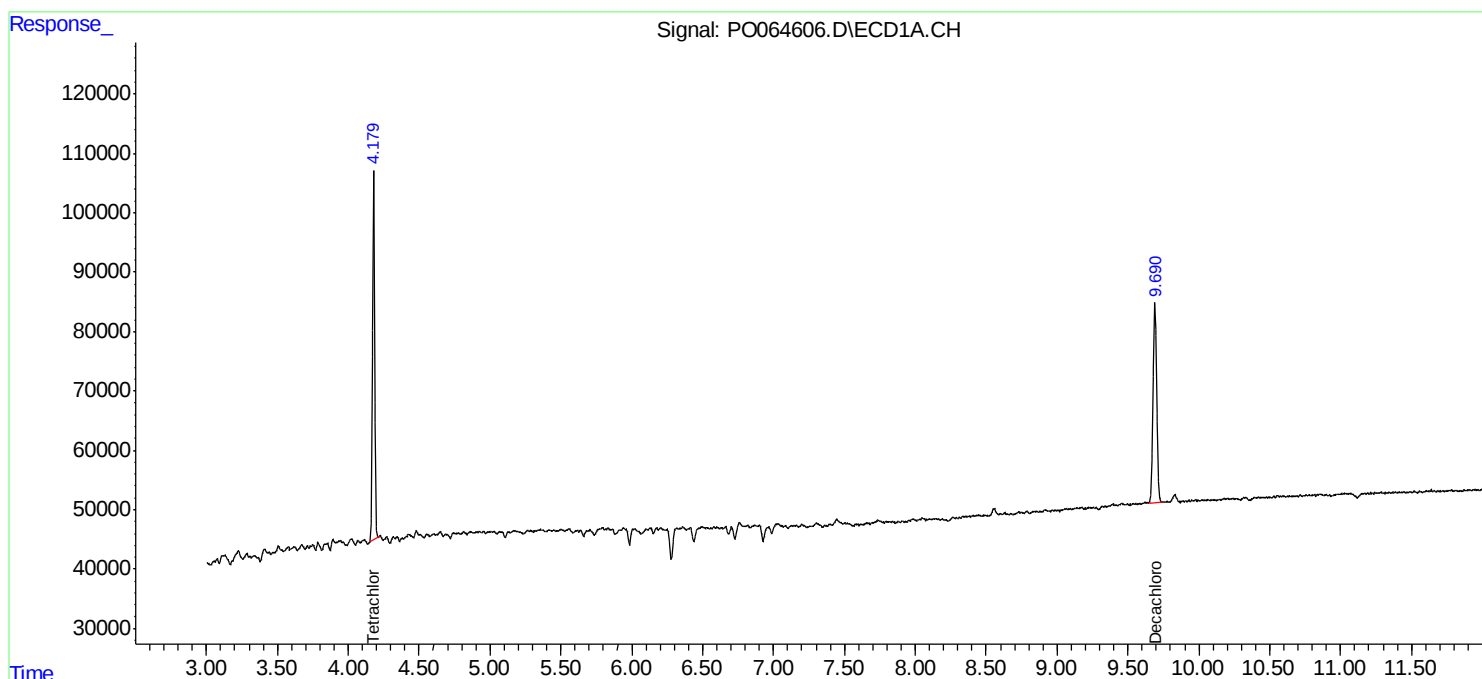

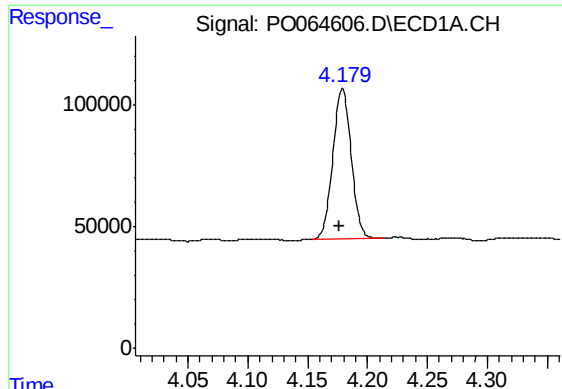


#1 Tetrachloro-m-xylene

R.T.: 4.179 min
Delta R.T.: 0.002 min
Response: 661440
Conc: 27.17 ng/ml m

Instrument :
ECD_O
ClientSampleId :
TP-1A-S


Manual Integrations
APPROVED

Ankita
12/16/2019 10:09:19 AM

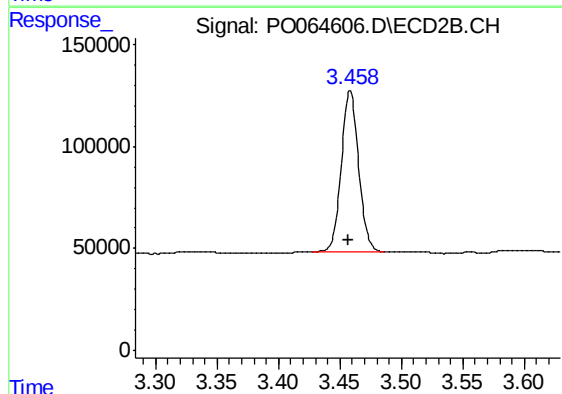


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.001 min
Response: 778711
Conc: 30.72 ng/ml m

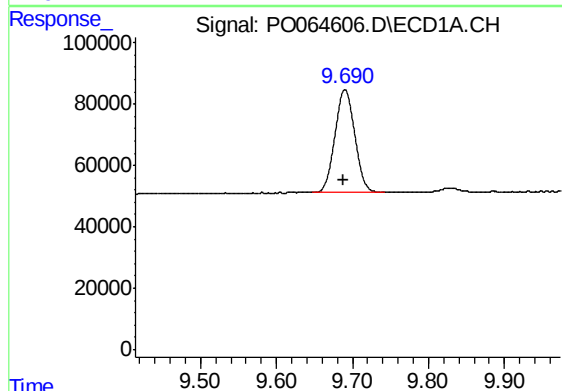

#2 Decachlorobiphenyl

R.T.: 9.690 min
Delta R.T.: 0.003 min
Response: 601917
Conc: 19.61 ng/ml m

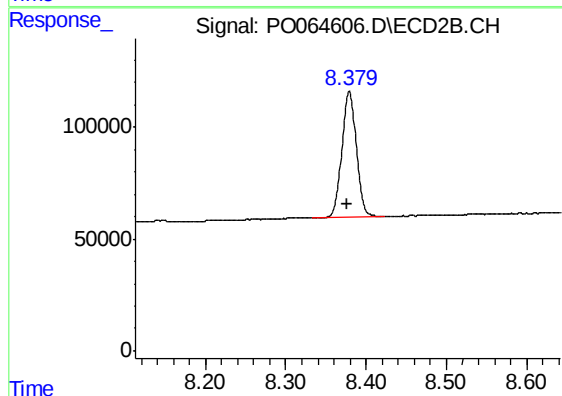

#2 Decachlorobiphenyl

R.T.: 8.379 min
Delta R.T.: 0.003 min
Response: 702061
Conc: 20.22 ng/ml