

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0121419\
 Data File : P0064620.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Dec 2019 18:41
 Operator : SM/AJ
 Sample : K6258-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MH-NEAR-THE-FRONT-DOOR-(4A)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 00:36:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0121319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Dec 13 08:19:24 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.180	3.458	505422	639325	20.761	25.221
2) SA Decachlor...	9.696	8.382	486209	592235	15.842	17.053

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO121419\
Data File : PO064620.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Dec 2019 18:41
Operator : SM/AJ
Sample : K6258-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MH-NEAR-THE-FRONT-DOOR-(4A)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 00:36:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO121319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Dec 13 08:19:24 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

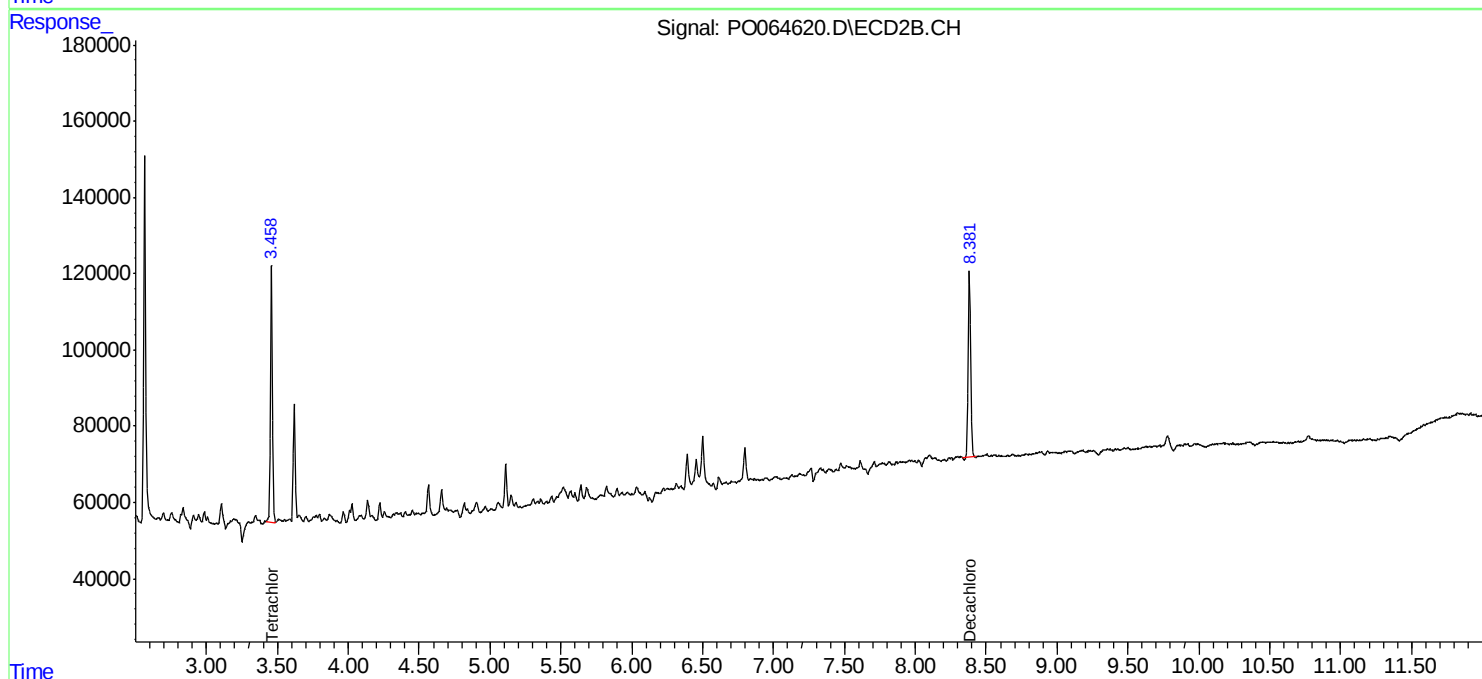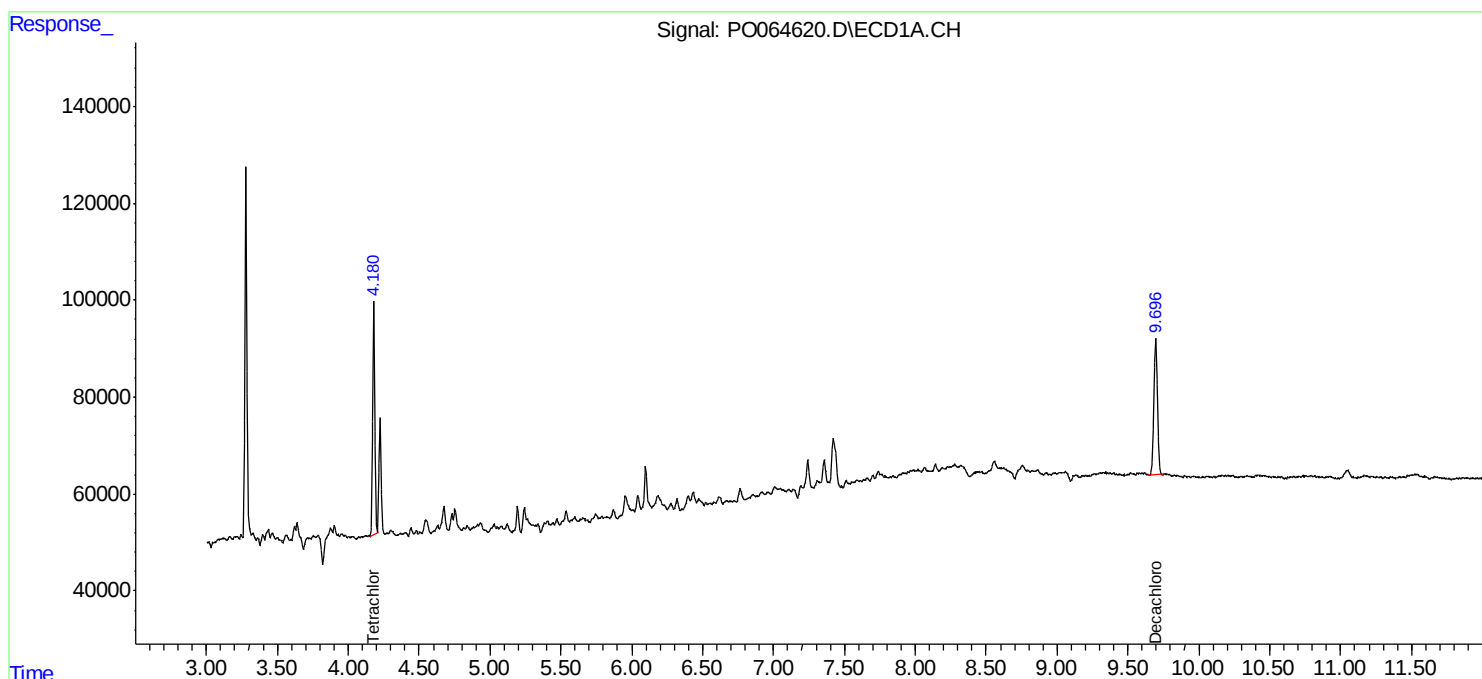


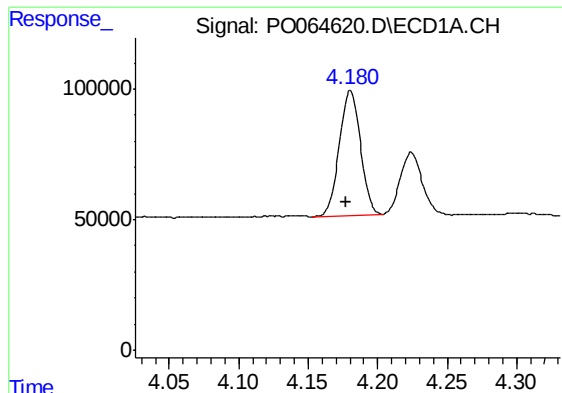

#1 Tetrachloro-m-xylene


R.T.: 4.180 min
Delta R.T.: 0.003 min
Response: 505422
Conc: 20.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
MH-NEAR-THE-FRONT-DOOR-(4A)

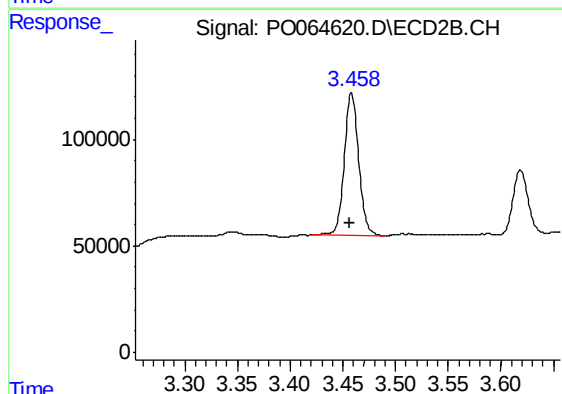


#1 Tetrachloro-m-xylene

R.T.: 3.458 min
Delta R.T.: 0.002 min
Response: 639325
Conc: 25.22 ng/ml

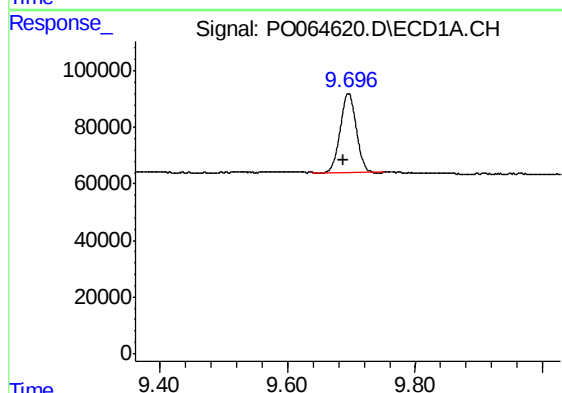

#2 Decachlorobiphenyl

R.T.: 9.696 min
Delta R.T.: 0.008 min
Response: 486209
Conc: 15.84 ng/ml

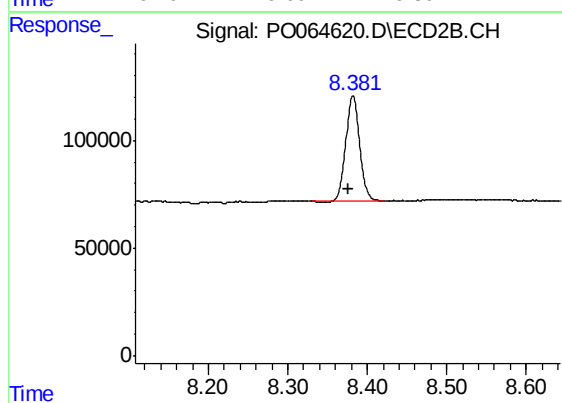

#2 Decachlorobiphenyl

R.T.: 8.382 min
Delta R.T.: 0.006 min
Response: 592235
Conc: 17.05 ng/ml